

SUPERVISOR TEST




NEW HARTFORD TOWN  
 POLICE DEPT  
 DATAMASTER dmt: 127606

Date: 01/07/2020

OPERATOR NAME:  
 MICHAEL T KOWALSKI  
 Permit #: 31077  
 Operator Agency/Dept: NEW HARTFORD TOWN PD  
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:50
INTERNAL STANDARD	VERIFIED	12:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.00	12:51
BLANK TEST	0.00	12:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.00	12:52
BLANK TEST	0.00	12:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.00	12:53
BLANK TEST	0.00	12:54

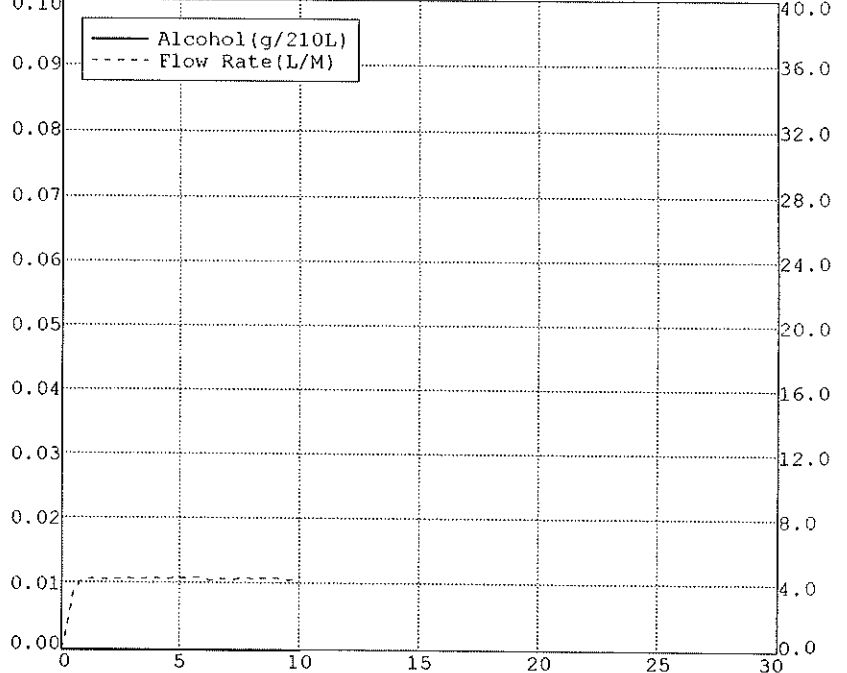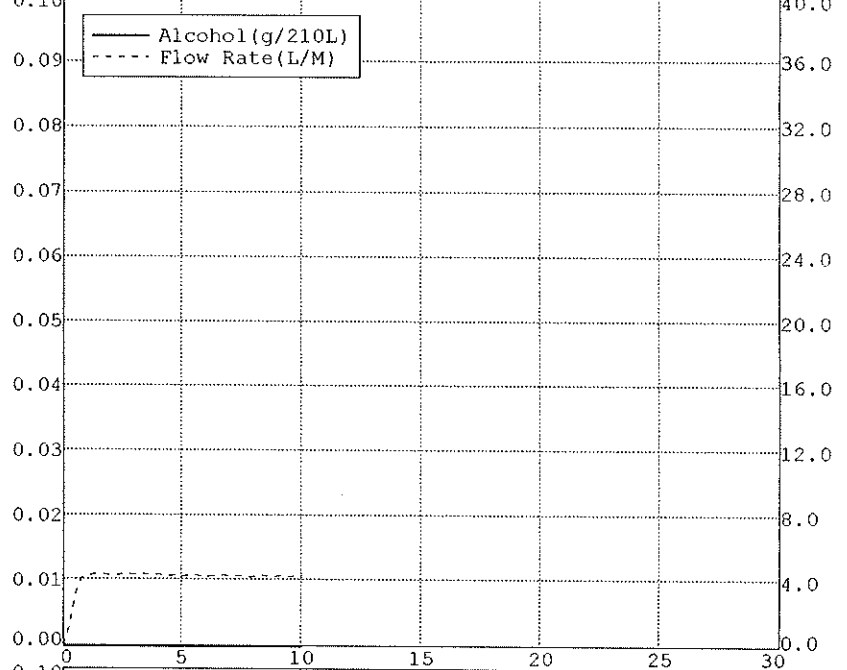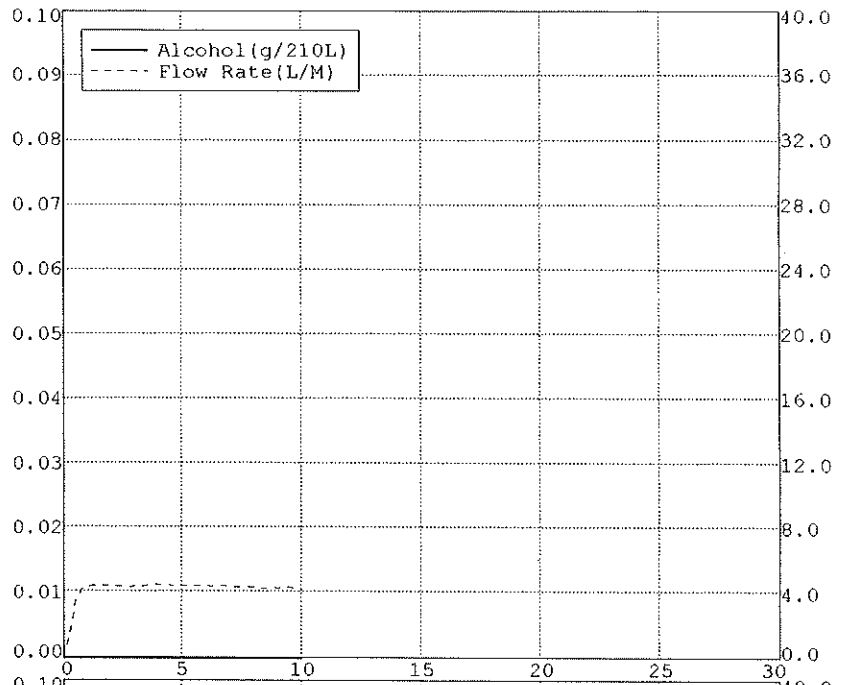

SUPERVISOR TEST




NEW HARTFORD TOWN  
POLICE DEPT  
DATAMASTER dmt: 127606

Date: 12/30/2019

OPERATOR NAME:  
MICHAEL T KOWALSKI  
Permit #: 31077  
Operator Agency/Dept: NEW HARTFORD TOWN PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:38
INTERNAL STANDARD	VERIFIED	11:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.00	11:39
BLANK TEST	0.00	11:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.00	11:40
BLANK TEST	0.00	11:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.00	11:41
BLANK TEST	0.00	11:42

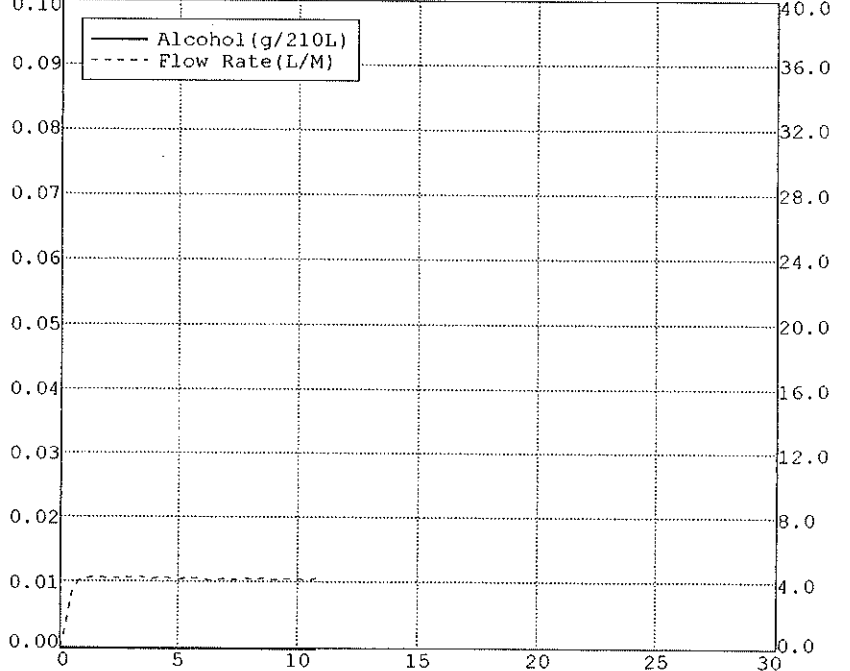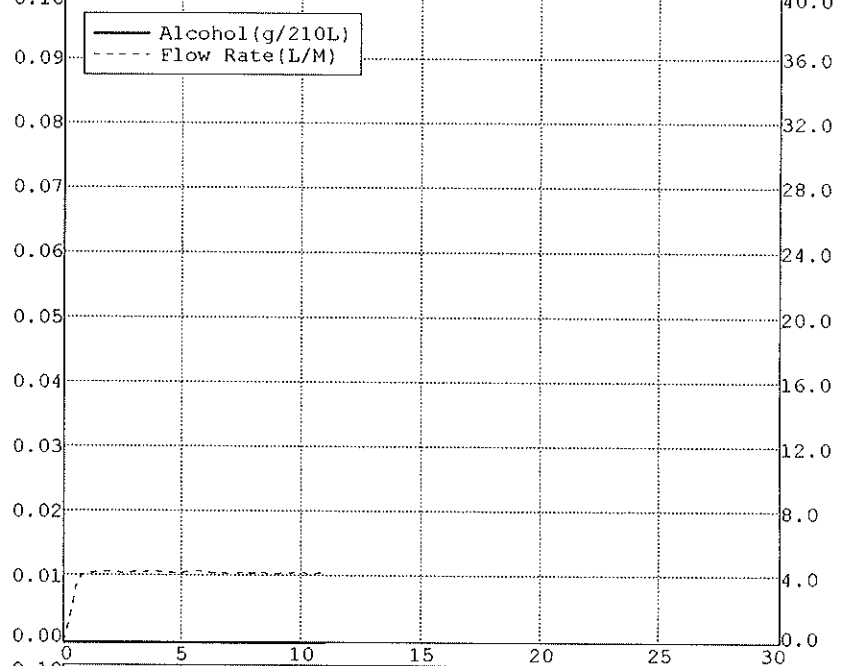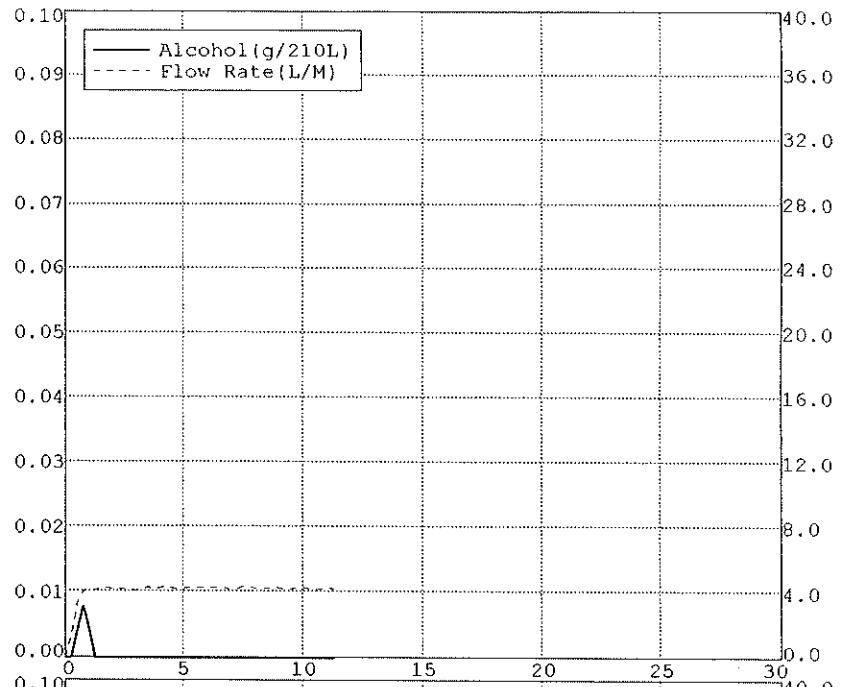

SUPERVISOR TEST

NEW HARTFORD TOWN  
POLICE DEPT  
DATAMASTER dmt: 127606

Date: 12/26/2019

OPERATOR NAME:  
MICHAEL T KOWALSKI  
Permit #: 31077  
Operator Agency/Dept: NEW HARTFORD TOWN PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:29
INTERNAL STANDARD	VERIFIED	21:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:29
BLANK TEST	0.00	21:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:31
BLANK TEST	0.00	21:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:32
BLANK TEST	0.00	21:33

