

SUPERVISOR TEST

LEA




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 06/10/2020

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:05
INTERNAL STANDARD	VERIFIED	18:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:05
BLANK TEST	0.00	18:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:06
BLANK TEST	0.00	18:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:07
BLANK TEST	0.00	18:08

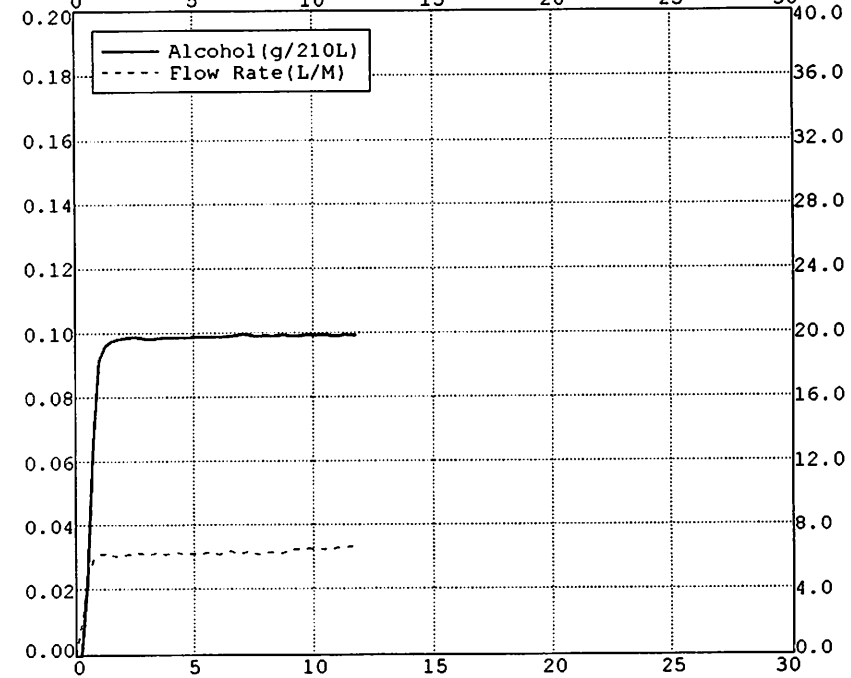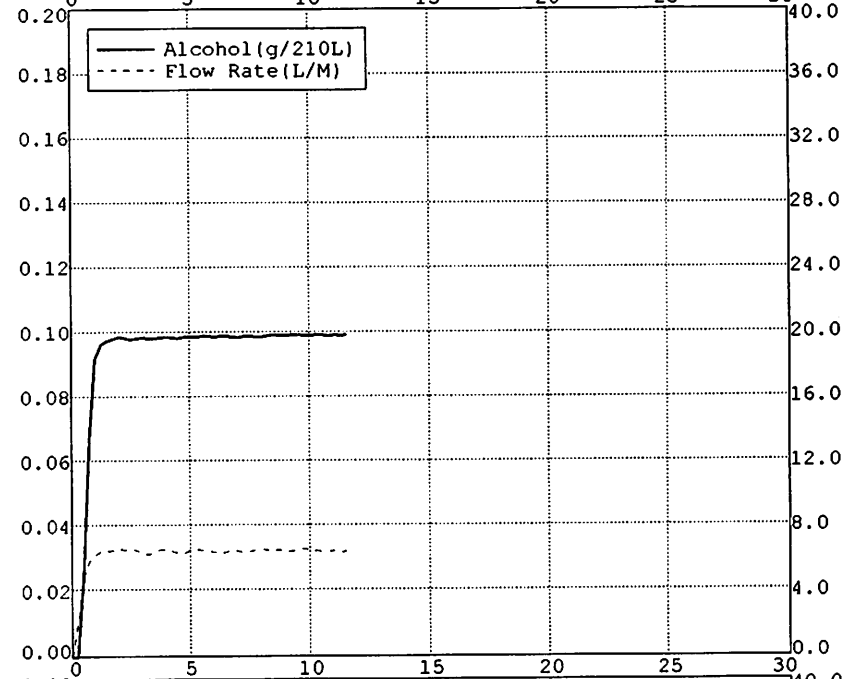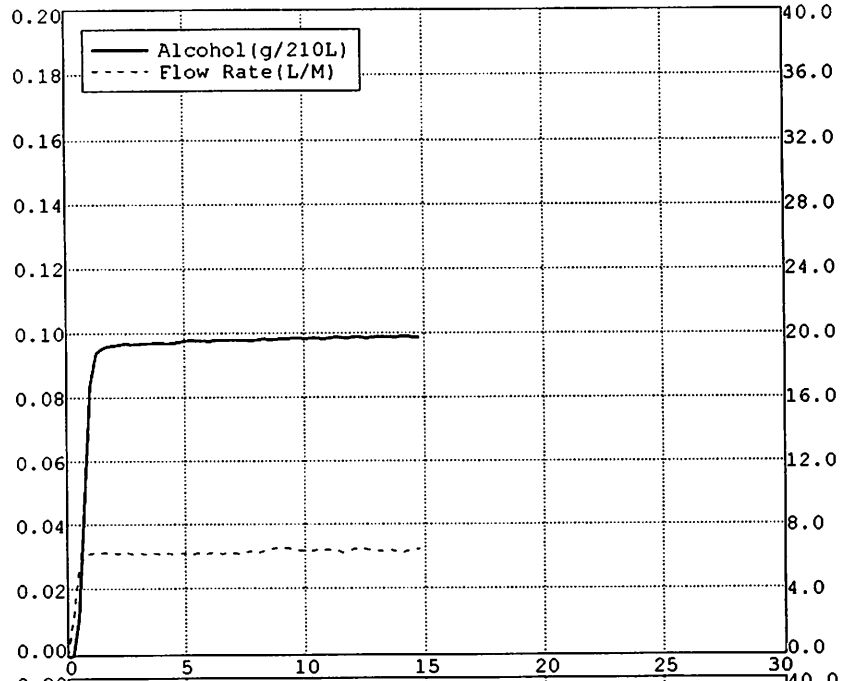

SUPERVISOR TEST

LATIC

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

LBS

Date: 06/17/2020

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:33
INTERNAL STANDARD	VERIFIED	23:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:33
BLANK TEST	0.00	23:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:35
BLANK TEST	0.00	23:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:36
BLANK TEST	0.00	23:37

