

SUPERVISOR TEST




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 07/04/2019

OPERATOR NAME:
MICHAEL P BAKER
Permit #: 44230
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:08
INTERNAL STANDARD	VERIFIED	01:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:09
BLANK TEST	0.00	01:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:10
BLANK TEST	0.00	01:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:11
BLANK TEST	0.00	01:12

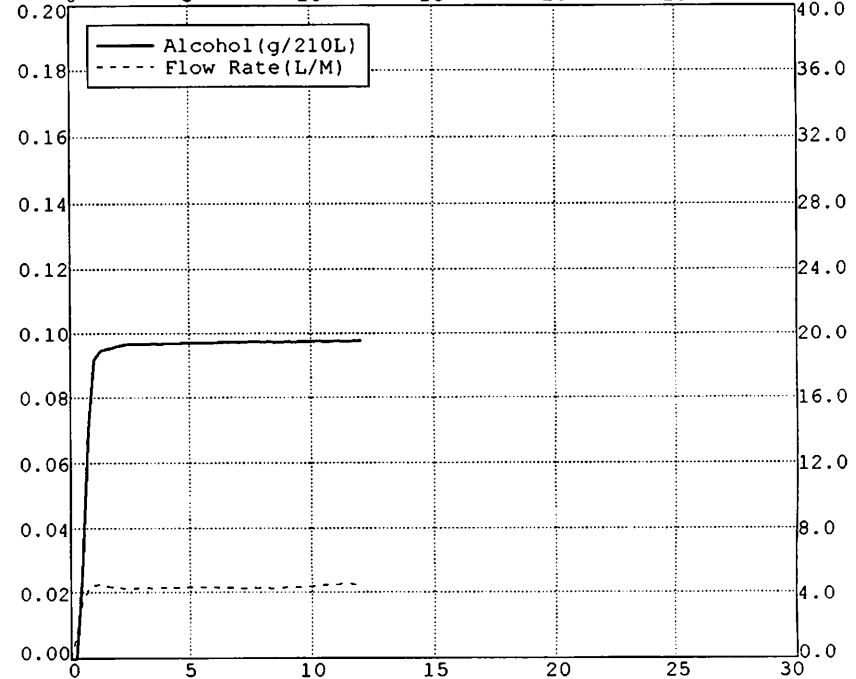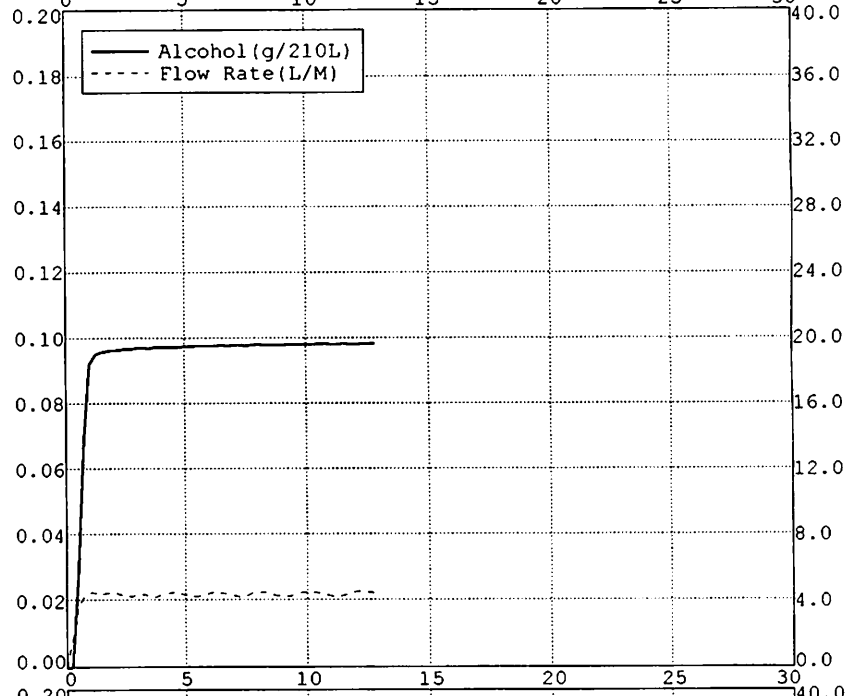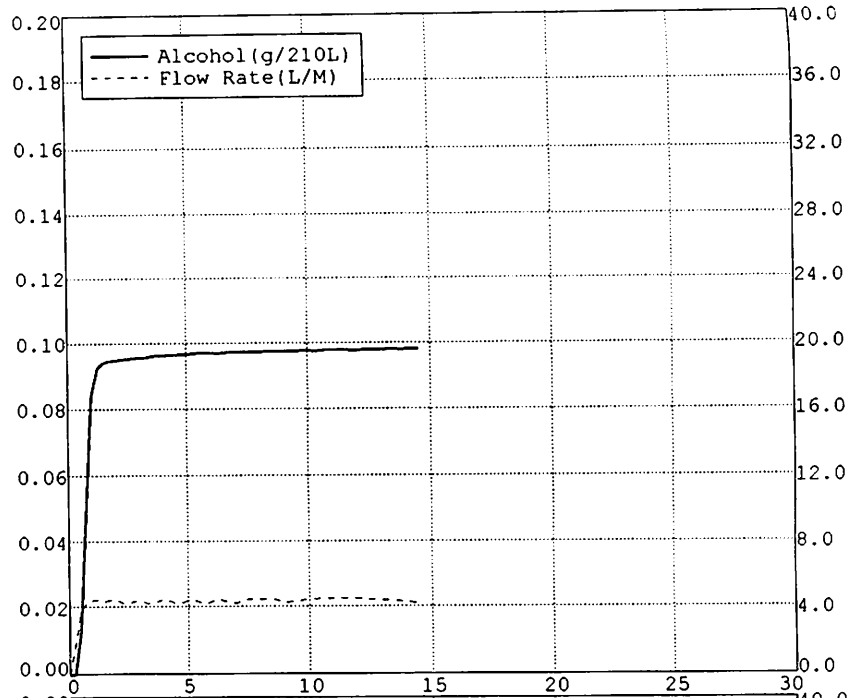

SUPERVISOR TEST

CFO




 ONEIDA CO.
 SHERIFF'S DEPT
 DATAMASTER dmt: 123906

Date: 07/10/2019

OPERATOR NAME:
 BRETT A GRABELDINGER
 Permit #: 46896
 Operator Agency/Dept: ONEIDA CO. SO
 Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:17
INTERNAL STANDARD	VERIFIED	23:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:17
BLANK TEST	0.00	23:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:19
BLANK TEST	0.00	23:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:20
BLANK TEST	0.00	23:21

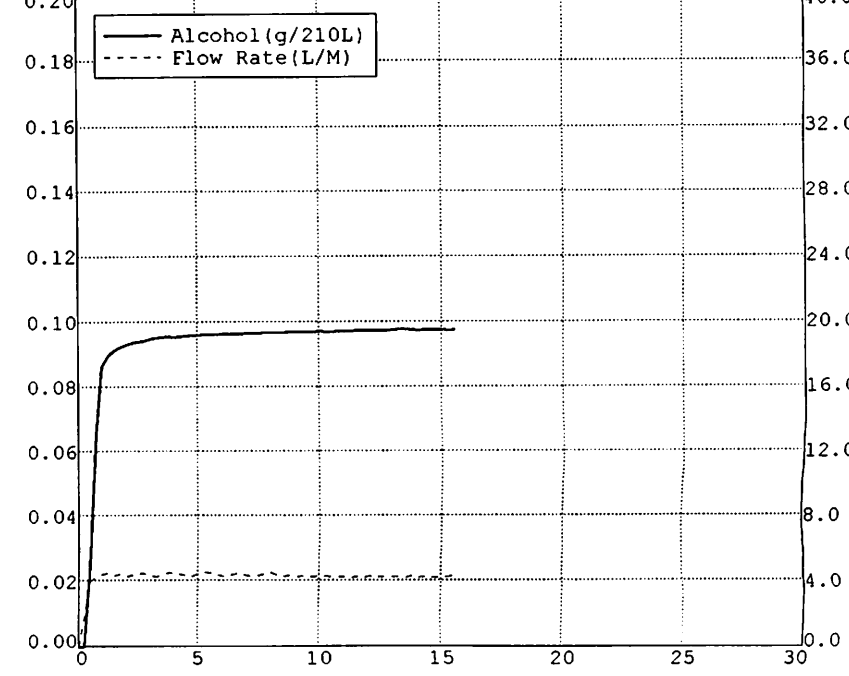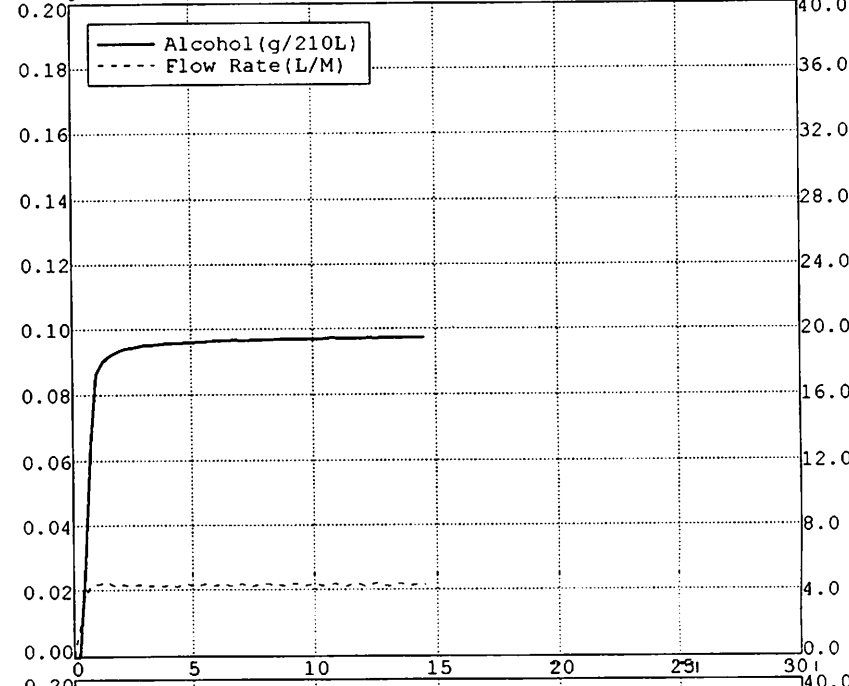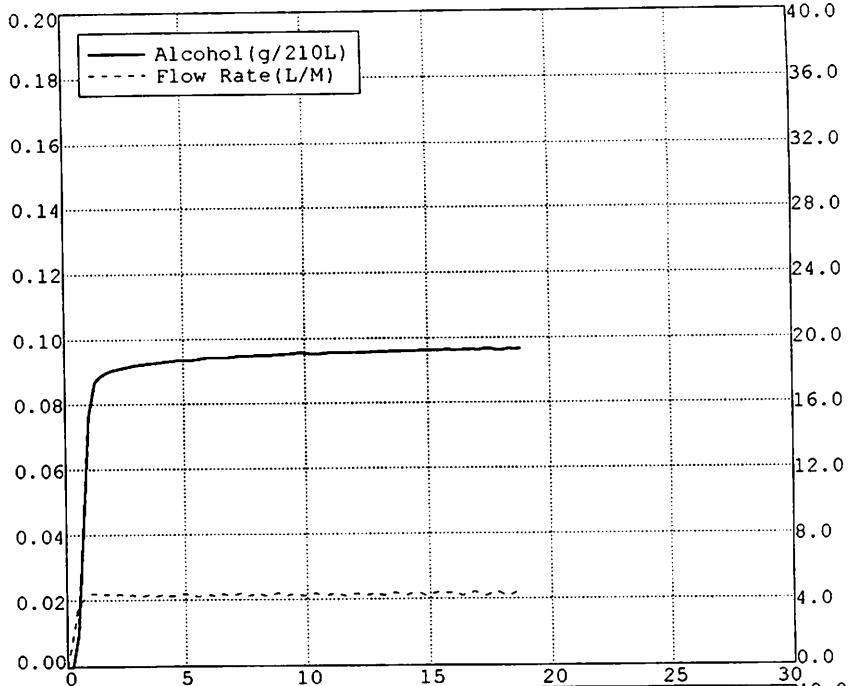

SUPERVISOR TEST

CFO



ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 07/19/2019

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:52
INTERNAL STANDARD	VERIFIED	00:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:53
BLANK TEST	0.00	00:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:54
BLANK TEST	0.00	00:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:55
BLANK TEST	0.00	00:56

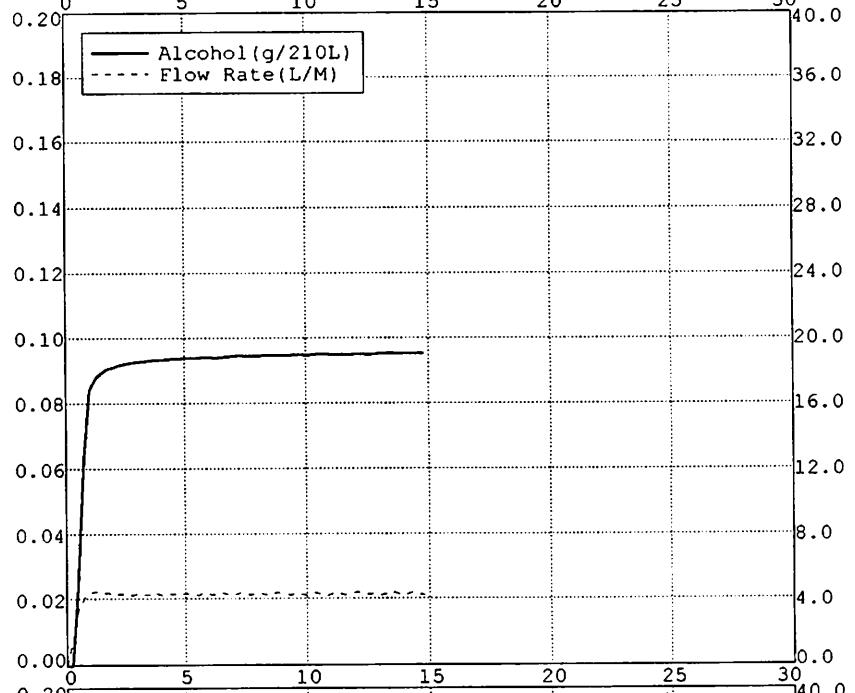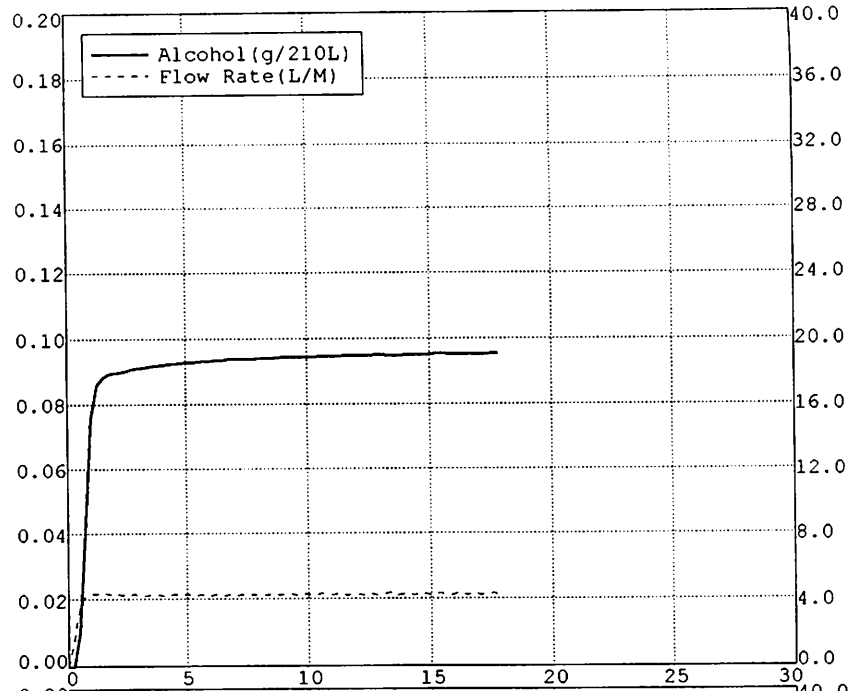

CFO

SUPERVISOR TEST




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 07/24/2019

OPERATOR NAME:
JOHN R BOWERS
Permit #: 46887
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:30
INTERNAL STANDARD	VERIFIED	22:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:31
BLANK TEST	0.00	22:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:32
BLANK TEST	0.00	22:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:33
BLANK TEST	0.00	22:34

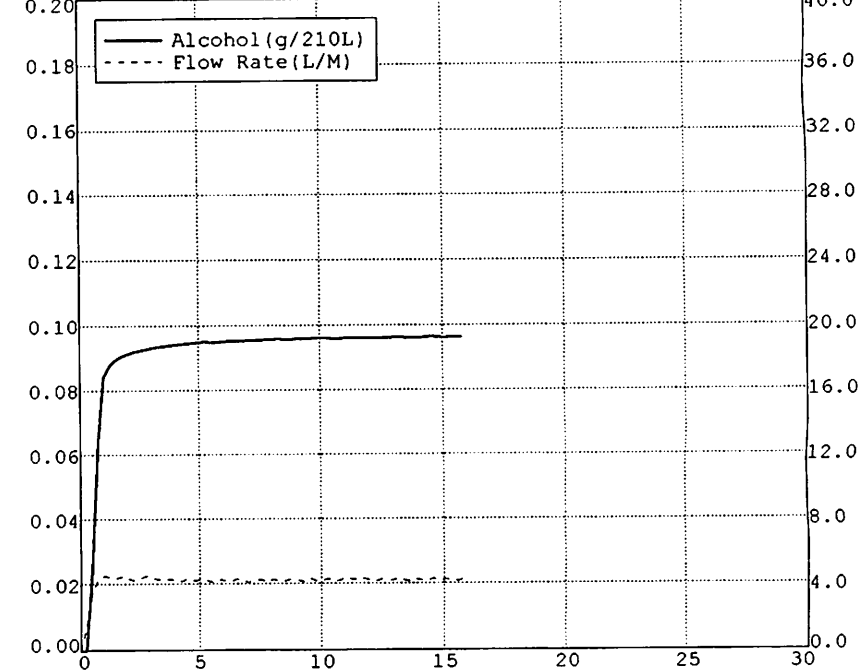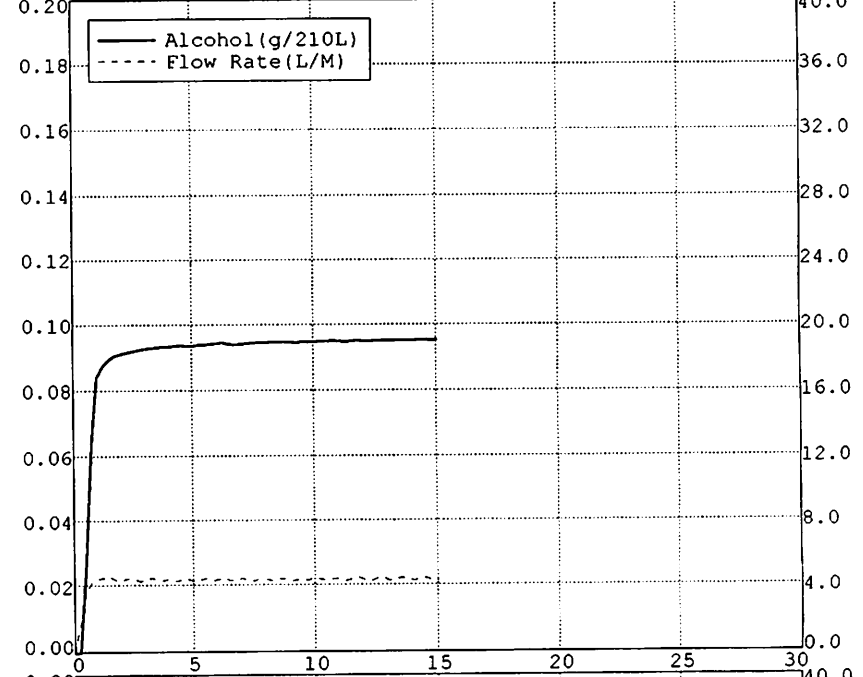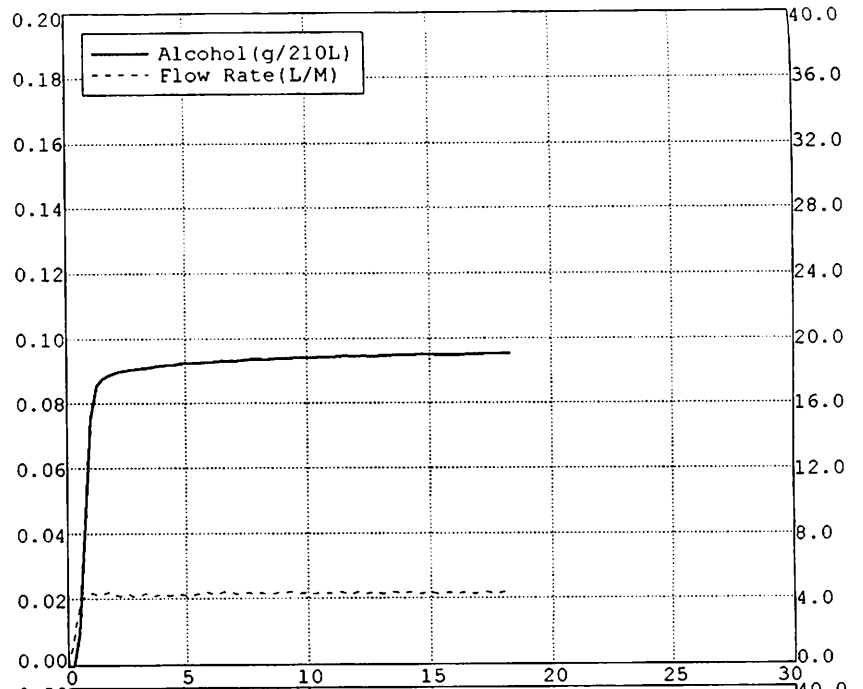

SOLUTION CHANGE




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 08/01/2019

OPERATOR NAME:
EDWARD F CONSTANTINE
Permit #: 45980
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:02
INTERNAL STANDARD	VERIFIED	21:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:03
BLANK TEST	0.00	21:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:04
BLANK TEST	0.00	21:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	21:05
BLANK TEST	0.00	21:06

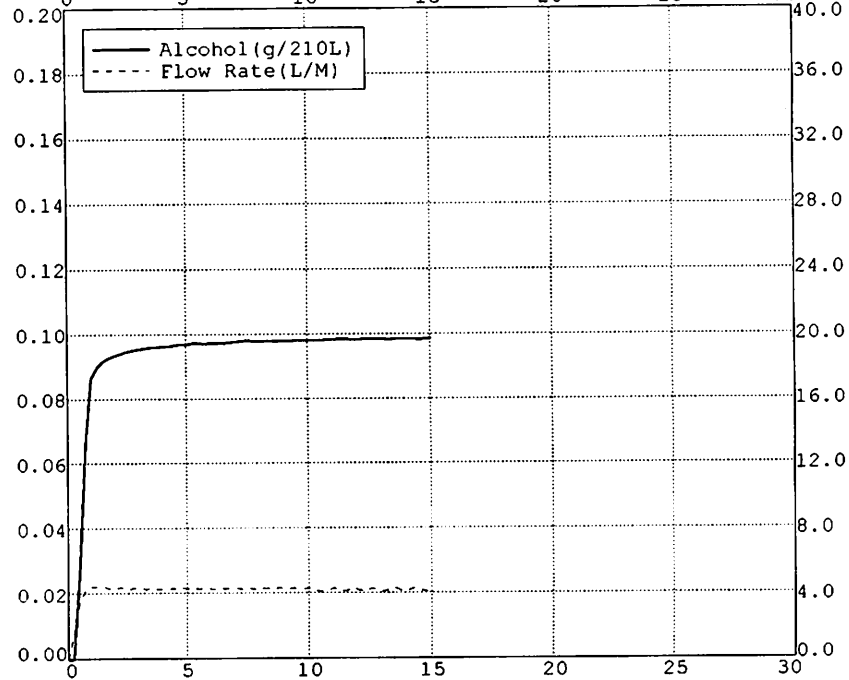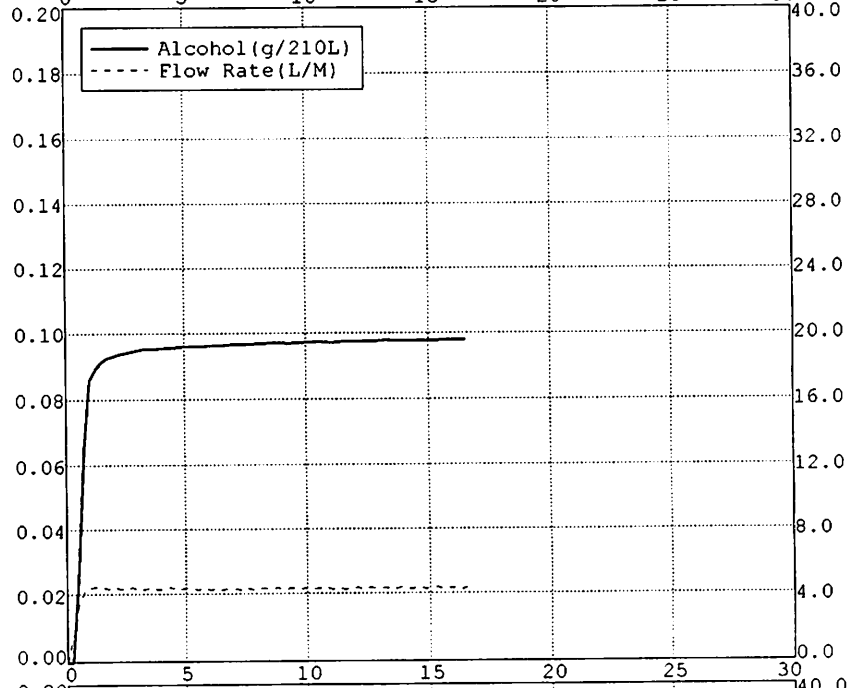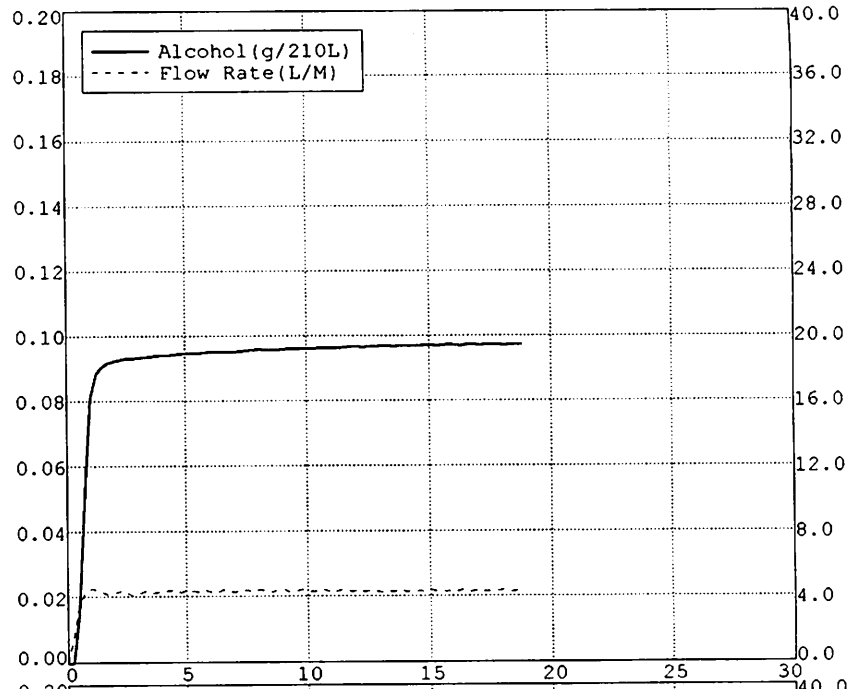

SUPERVISOR TEST

CFO




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 08/07/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:30
INTERNAL STANDARD	VERIFIED	19:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:31
BLANK TEST	0.00	19:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:32
BLANK TEST	0.00	19:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:33
BLANK TEST	0.00	19:34

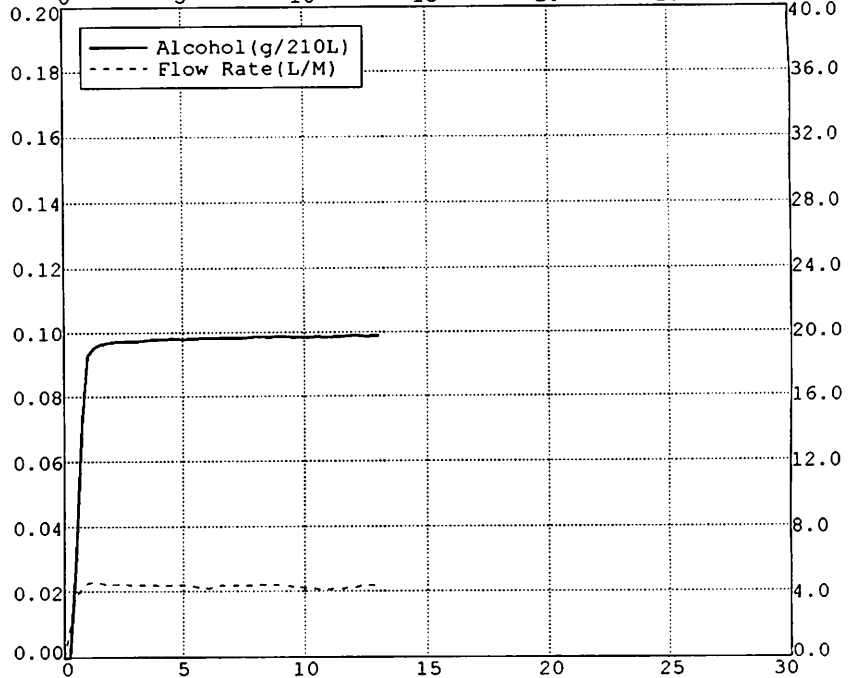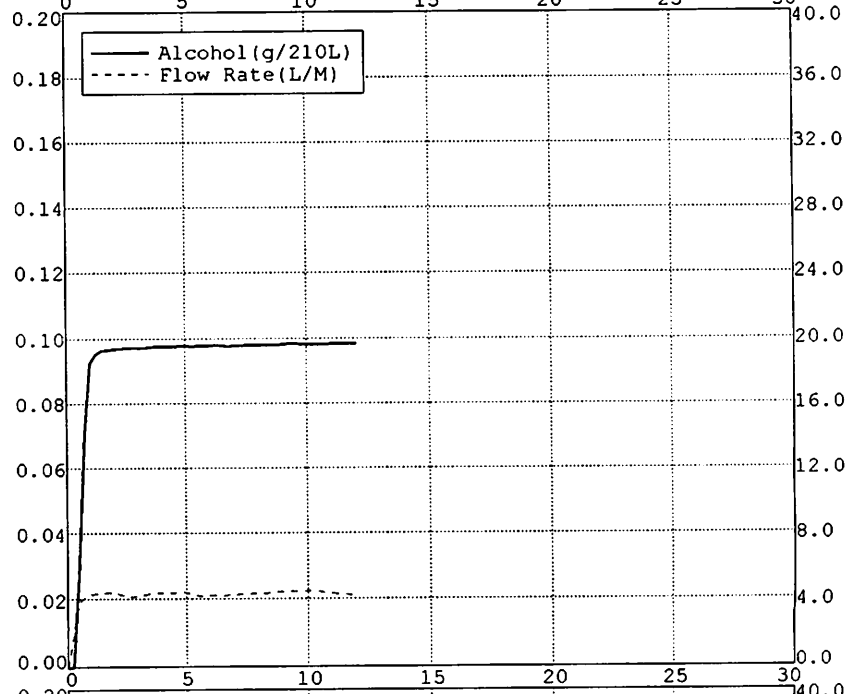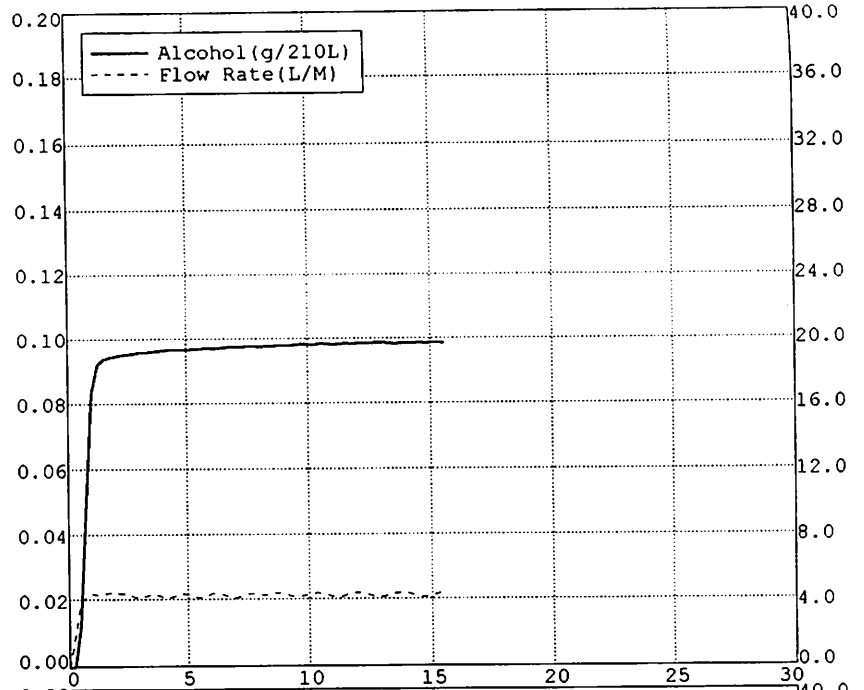

CFO

SUPERVISOR TEST




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 08/14/2019

OPERATOR NAME:
JOHN R BOWERS
Permit #: 46887
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:54
INTERNAL STANDARD	VERIFIED	22:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:54
BLANK TEST	0.00	22:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:56
BLANK TEST	0.00	22:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:57
BLANK TEST	0.00	22:58

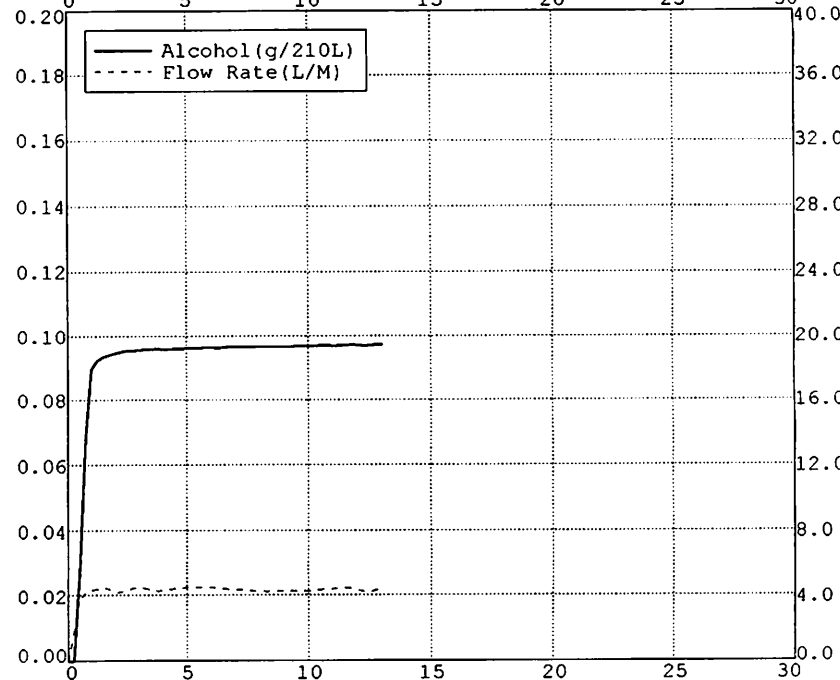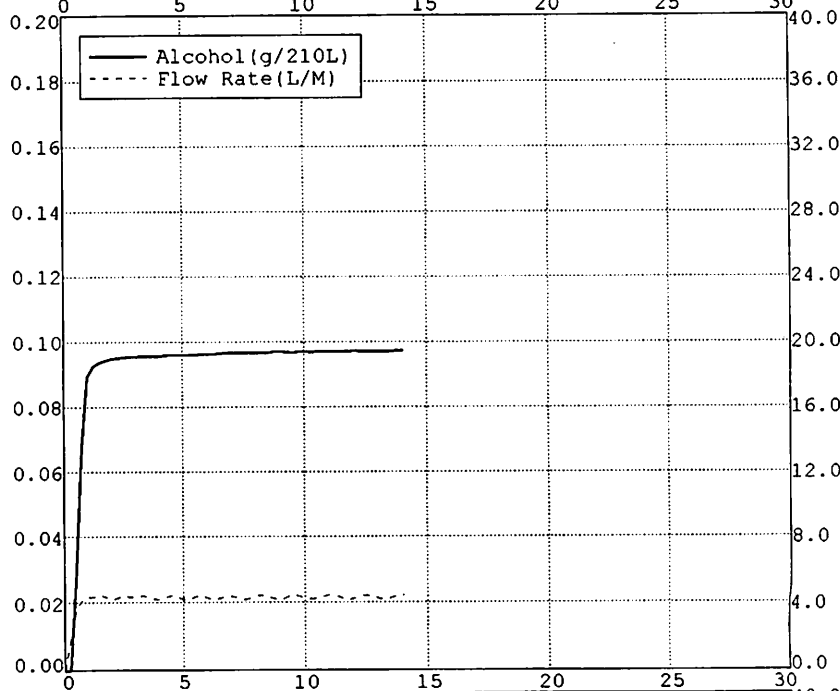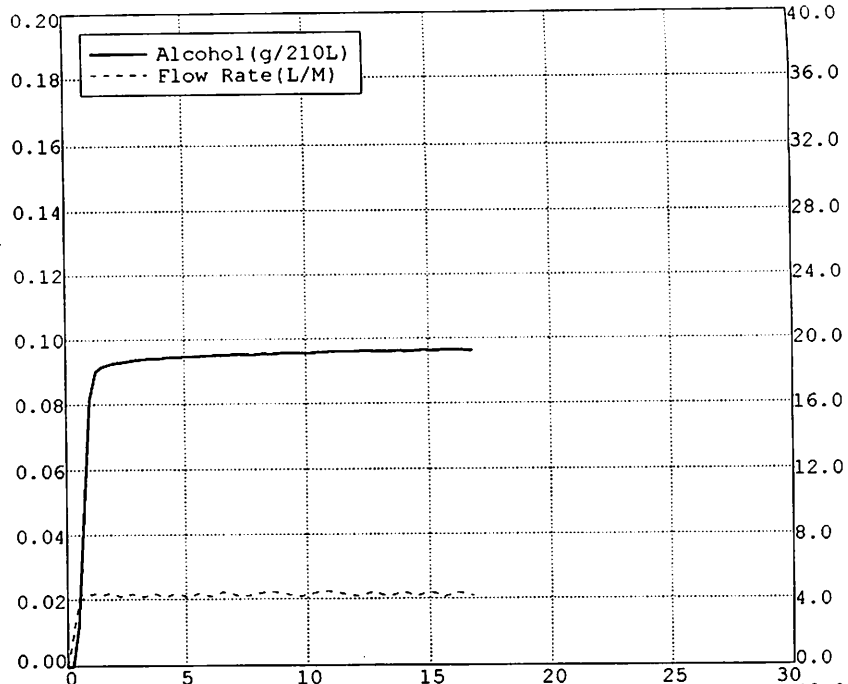

SUPERVISOR TEST




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 08/21/2019

OPERATOR NAME:
JASON L OSIKA
Permit #: 35567
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:05
INTERNAL STANDARD	VERIFIED	21:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:05
BLANK TEST	0.00	21:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:06
BLANK TEST	0.00	21:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:08
BLANK TEST	0.00	21:08

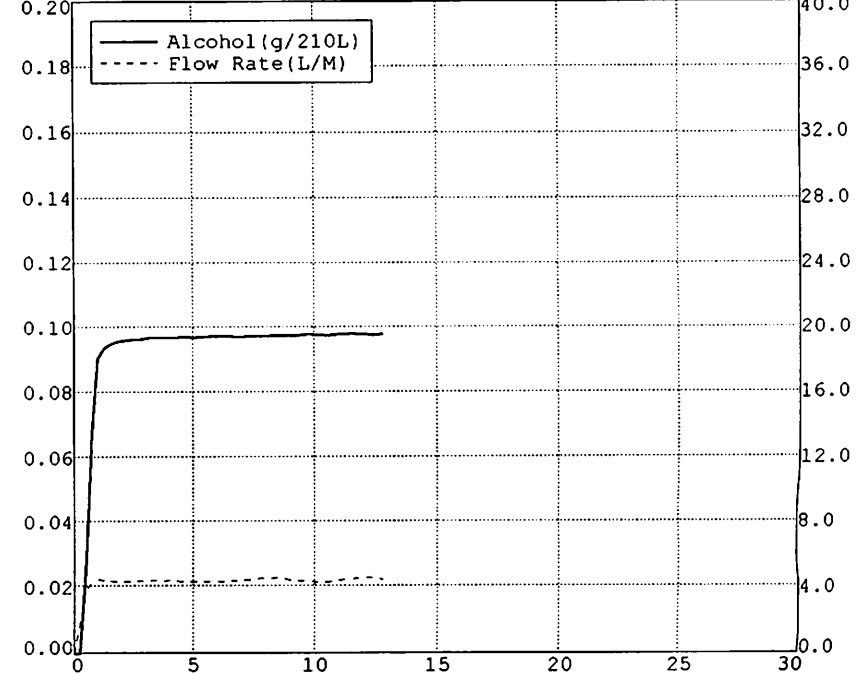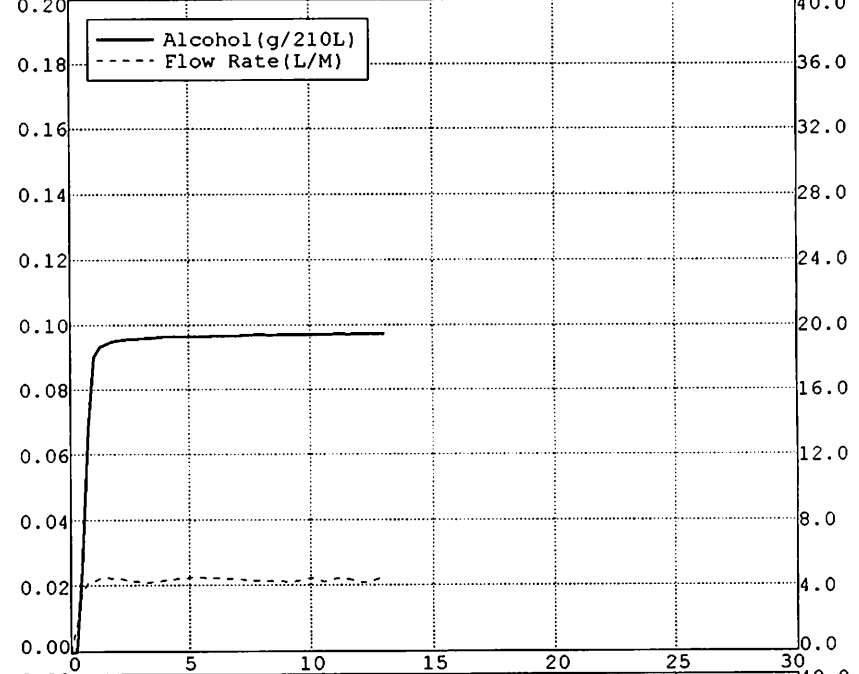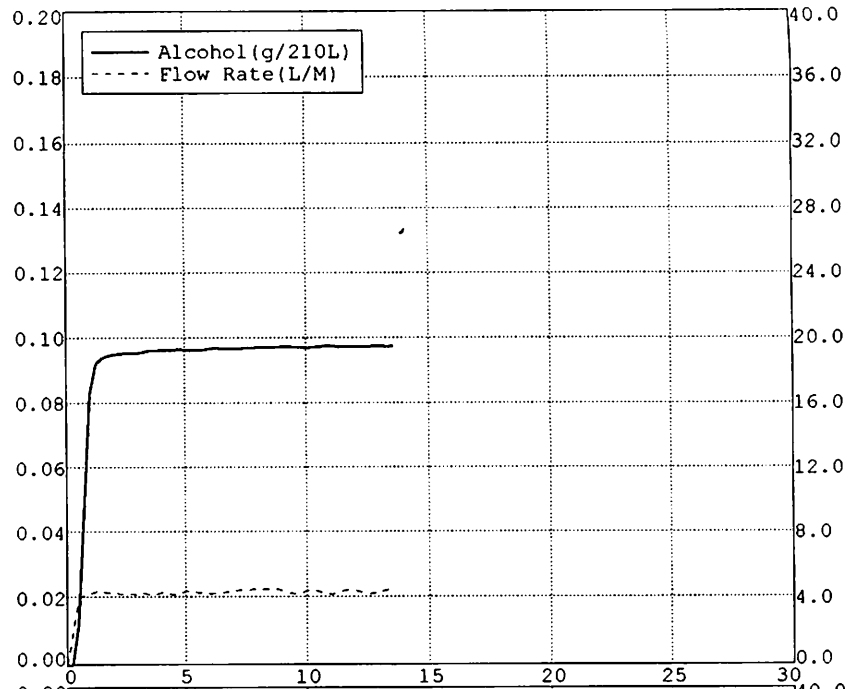

SUPERVISOR TEST

CFO




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 08/28/2019

OPERATOR NAME:
JOHN R BOWERS
Permit #: 46887
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:52
INTERNAL STANDARD	VERIFIED	22:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:52
BLANK TEST	0.00	22:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:53
BLANK TEST	0.00	22:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:54
BLANK TEST	0.00	22:55

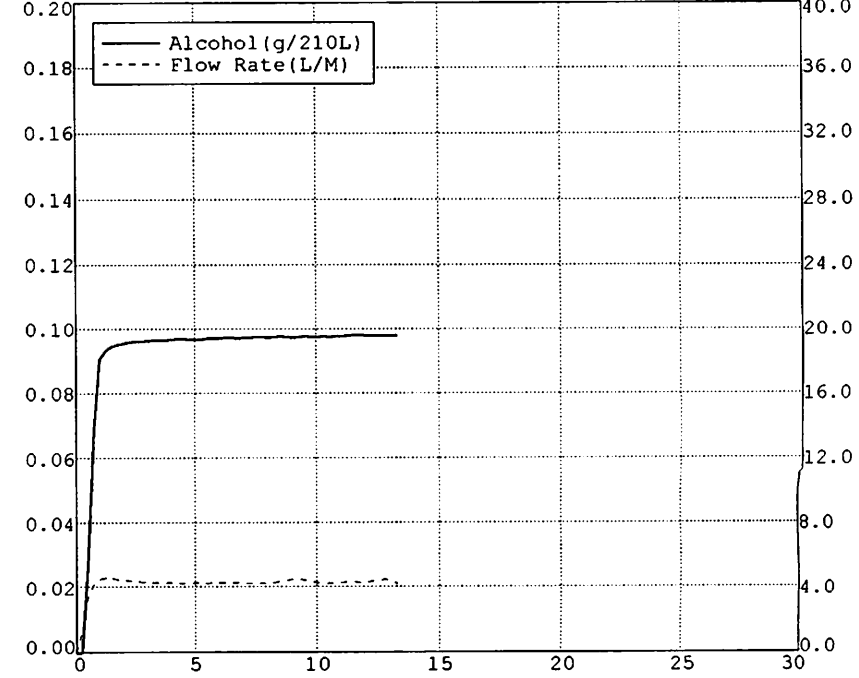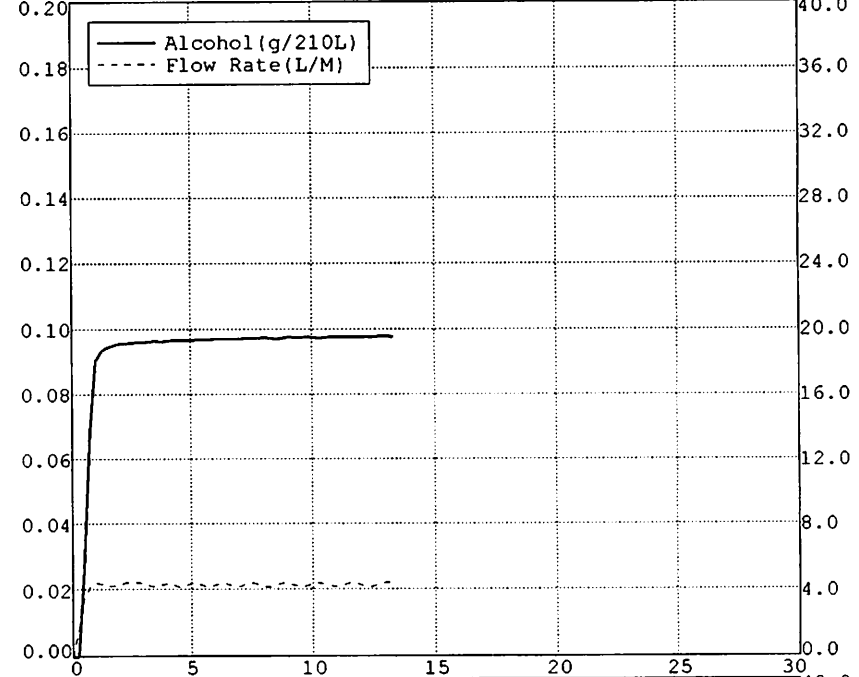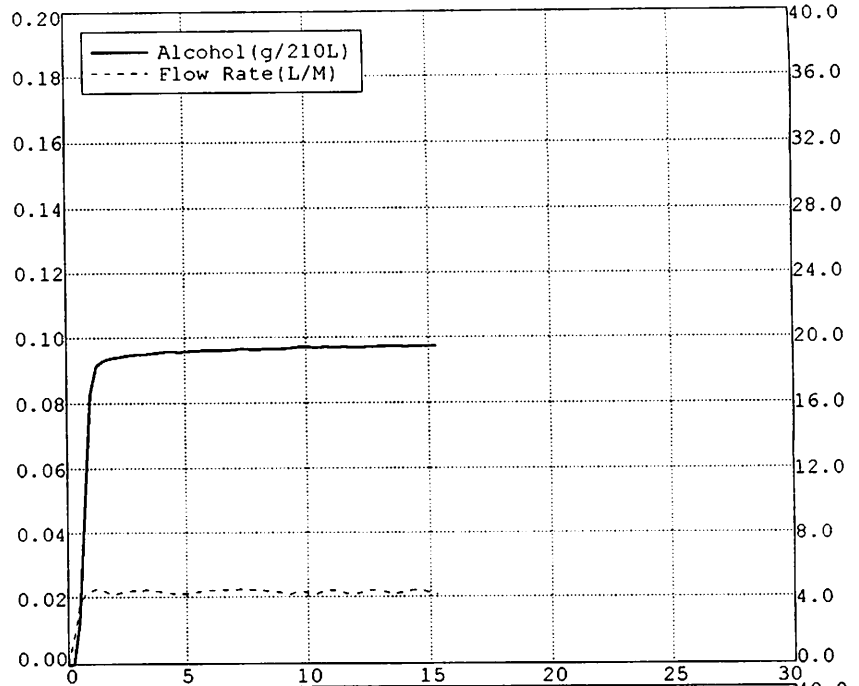

SUPERVISOR TEST

CFO




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 09/01/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:05
INTERNAL STANDARD	VERIFIED	21:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:06
BLANK TEST	0.00	21:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:07
BLANK TEST	0.00	21:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:08
BLANK TEST	0.00	21:09

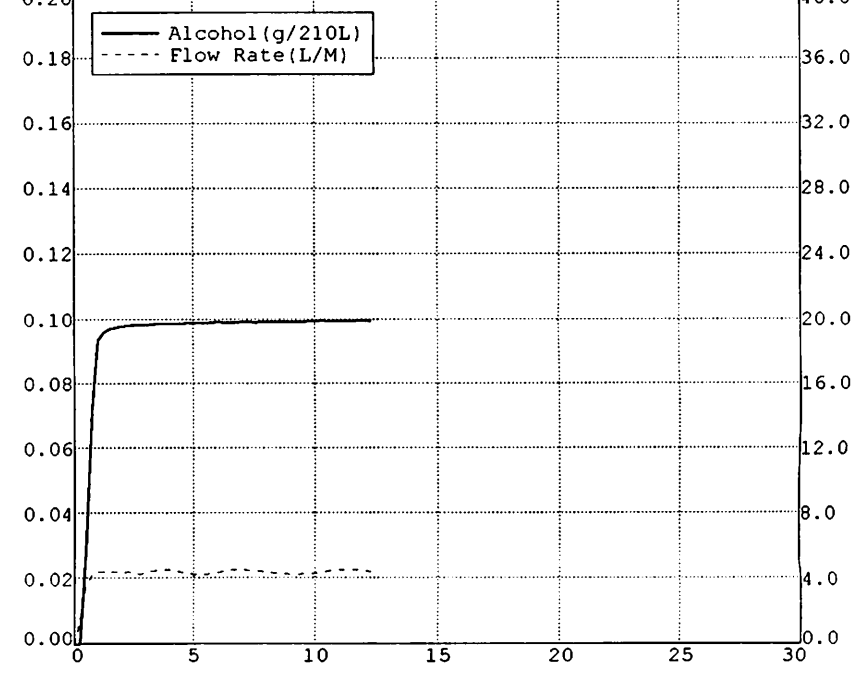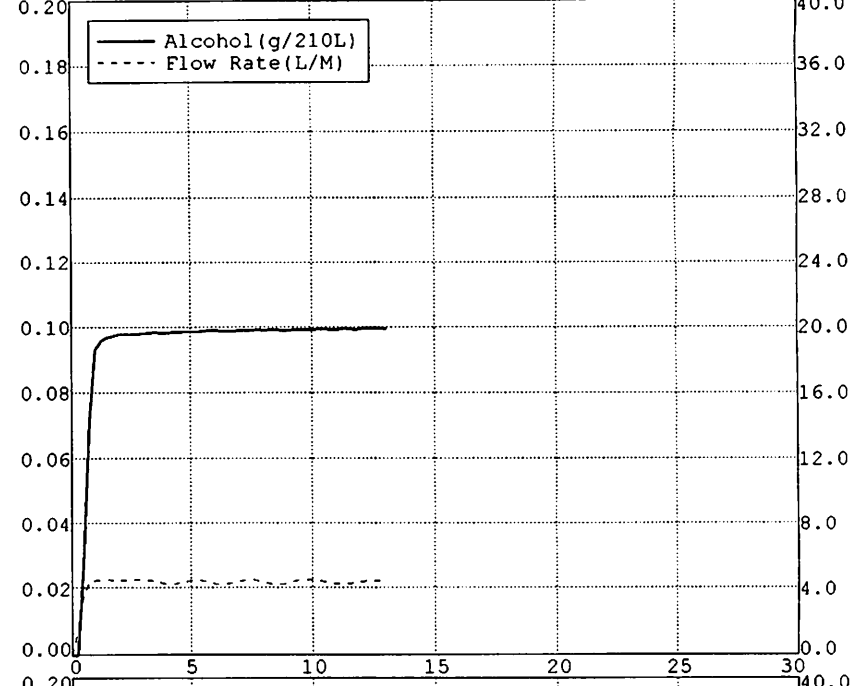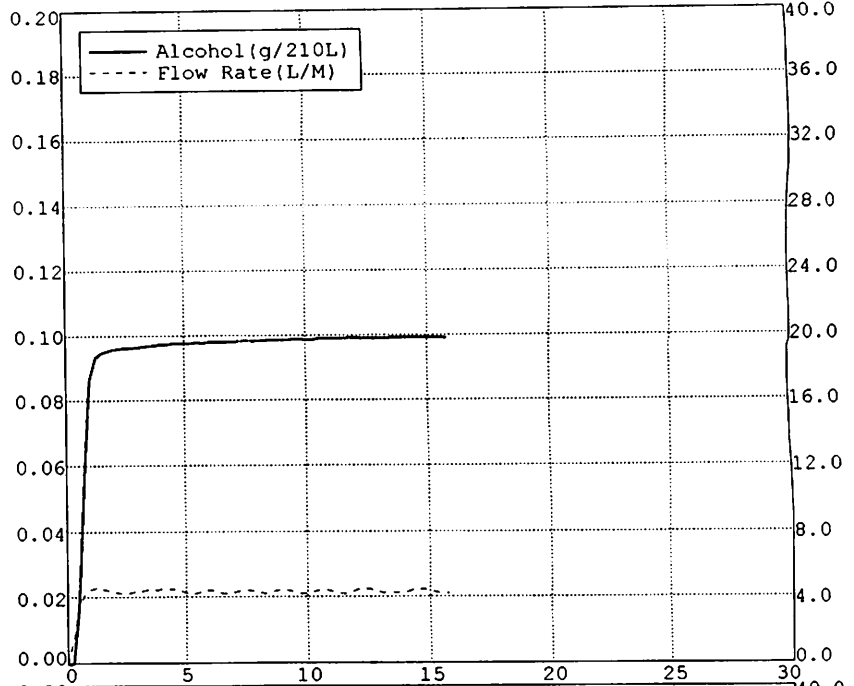

SUPERVISOR TEST **CFO**




ONEIDA CO.
 SHERIFF'S DEPT
 DATAMASTER dmt: 123906

Date: 09/04/2019

OPERATOR NAME:
 JOHN R BOWERS
 Permit #: 46887
 Operator Agency/Dept: ONEIDA CO. SO
 Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:31
INTERNAL STANDARD	VERIFIED	19:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:31
BLANK TEST	0.00	19:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:33
BLANK TEST	0.00	19:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:34
BLANK TEST	0.00	19:35

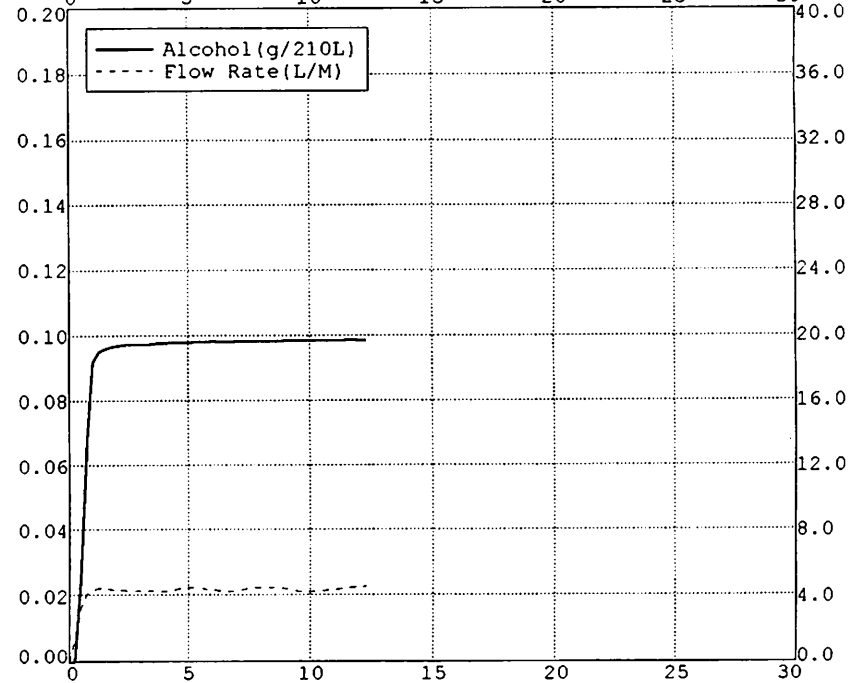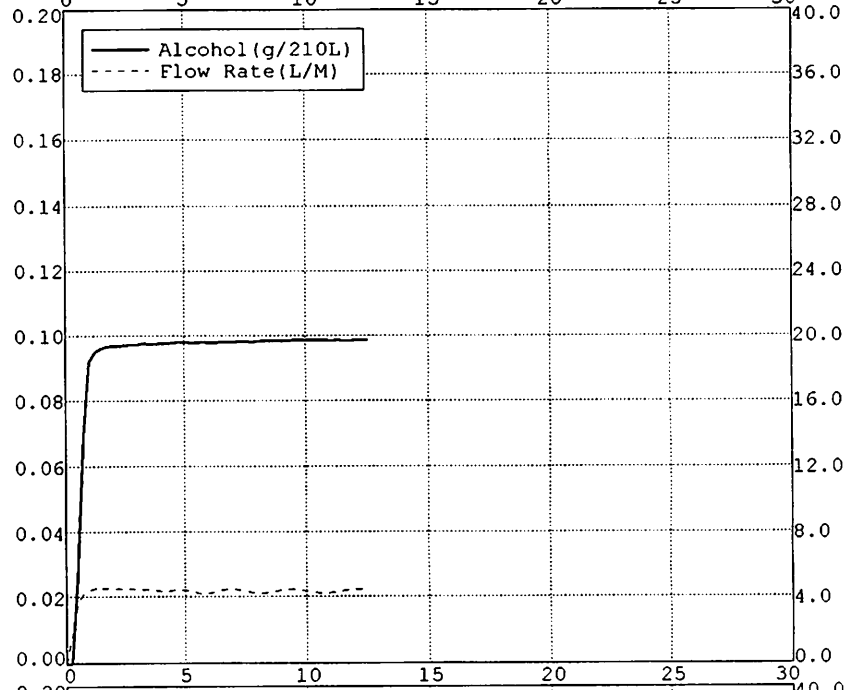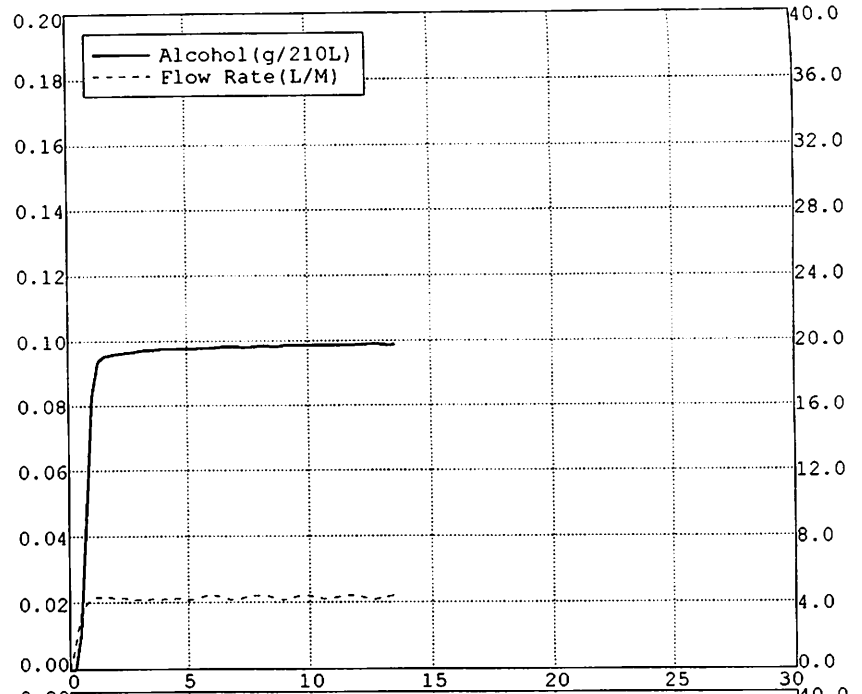

SUPERVISOR TEST

Cfo




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 09/11/2019

OPERATOR NAME:
JOHN R BOWERS
Permit #: 46887
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:15
INTERNAL STANDARD	VERIFIED	22:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:16
BLANK TEST	0.00	22:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:17
BLANK TEST	0.00	22:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:18
BLANK TEST	0.00	22:19

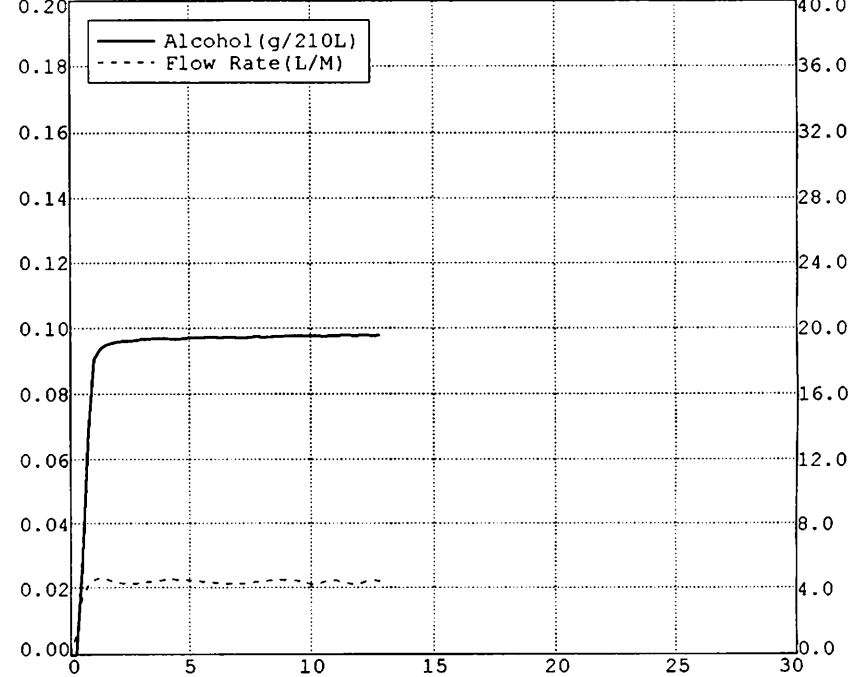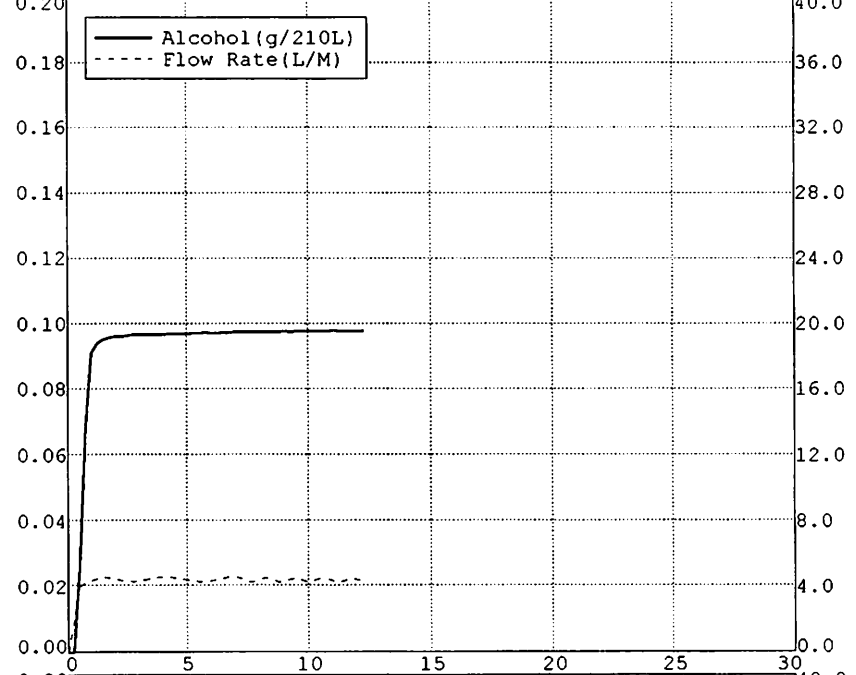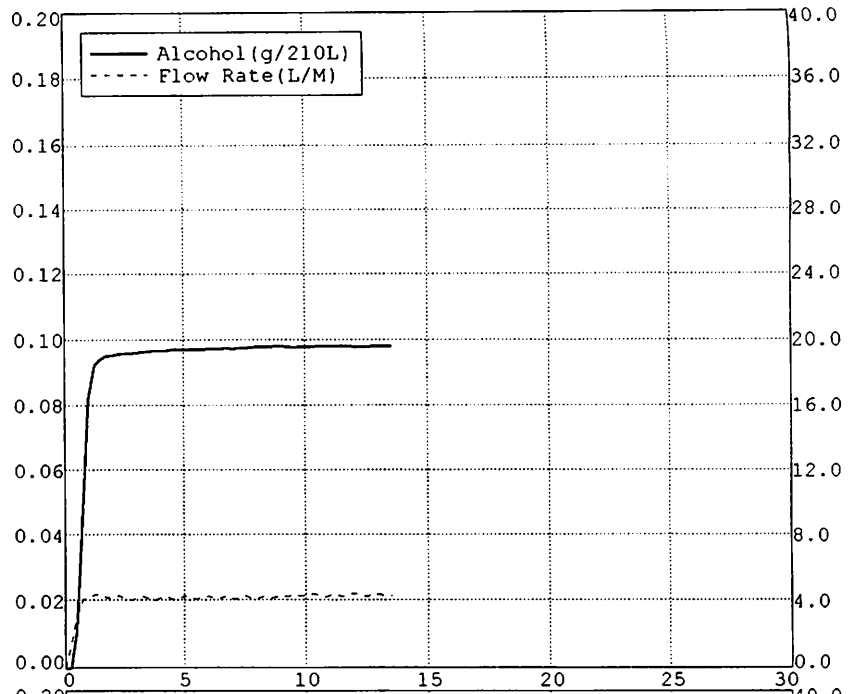

SUPERVISOR TEST

CFU




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 09/19/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:26
INTERNAL STANDARD	VERIFIED	03:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:26
BLANK TEST	0.00	03:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:27
BLANK TEST	0.00	03:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:28
BLANK TEST	0.00	03:29

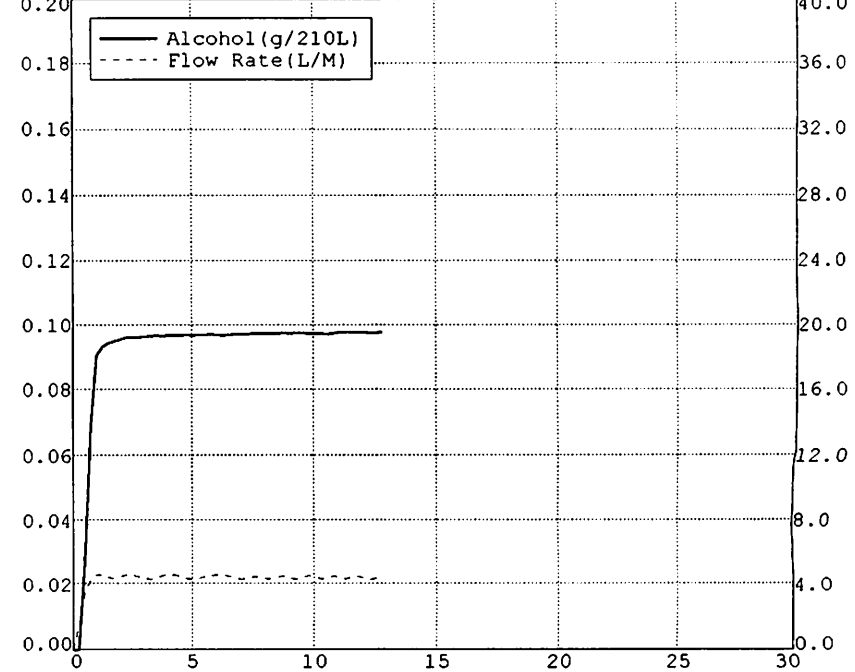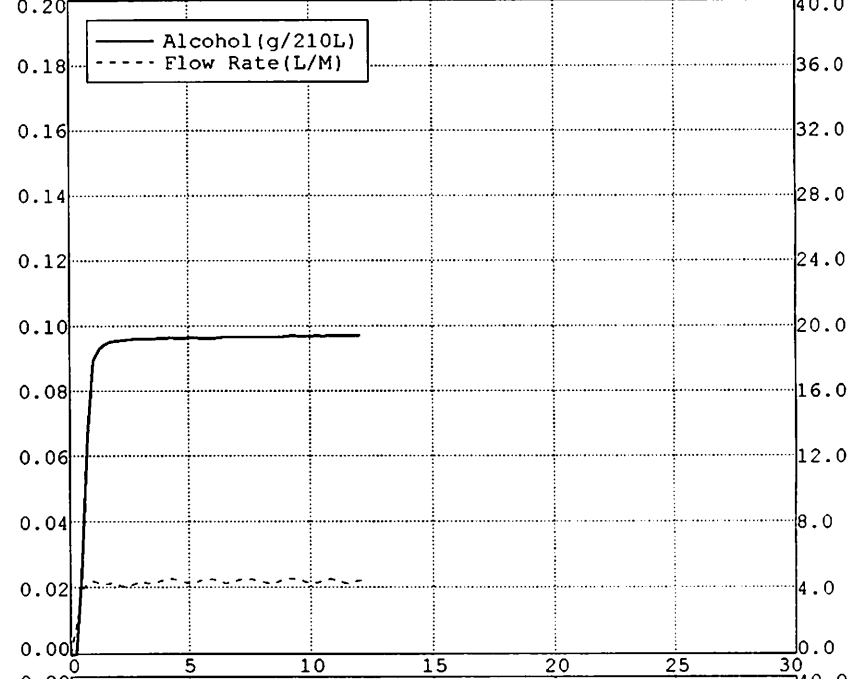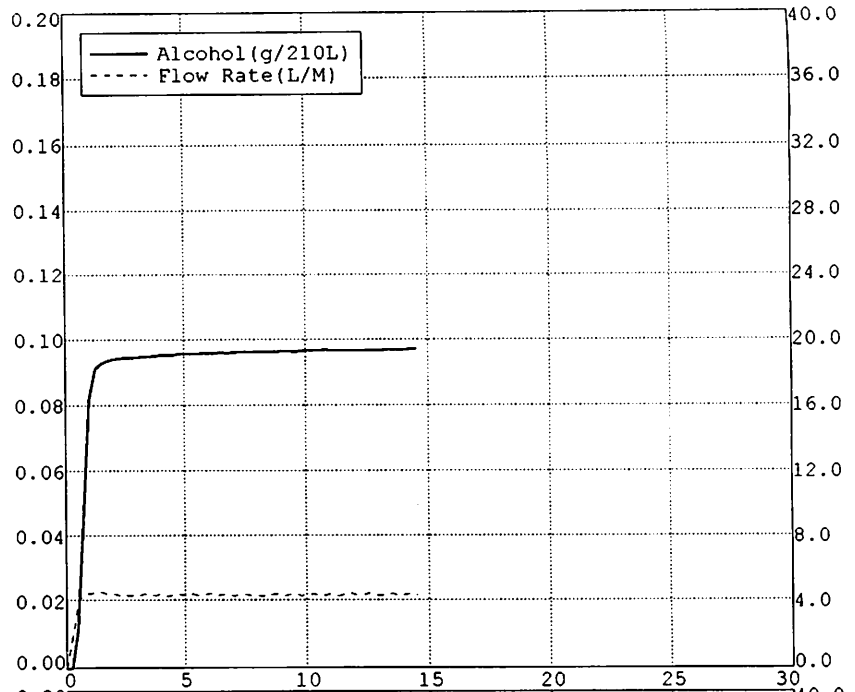

SUPERVISOR TEST

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906




LATIC
CFC

Date: 09/26/2019

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:17
INTERNAL STANDARD	VERIFIED	02:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:17
BLANK TEST	0.00	02:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:18
BLANK TEST	0.00	02:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:20
BLANK TEST	0.00	02:21

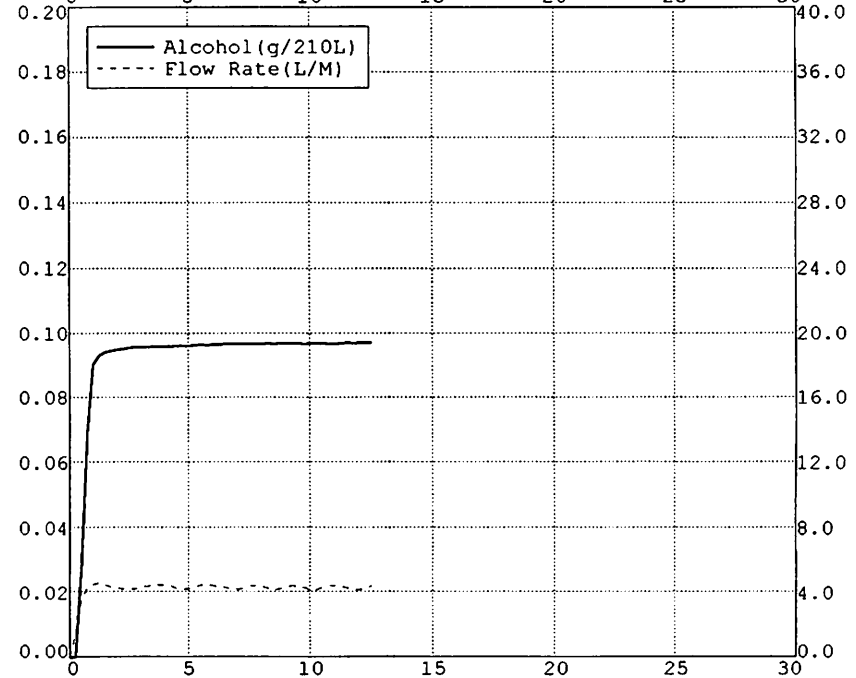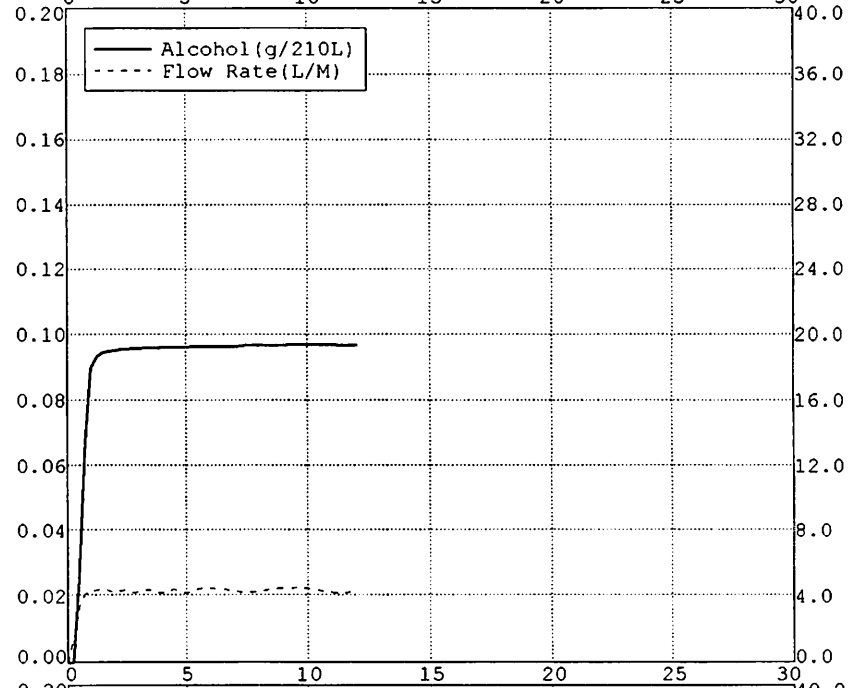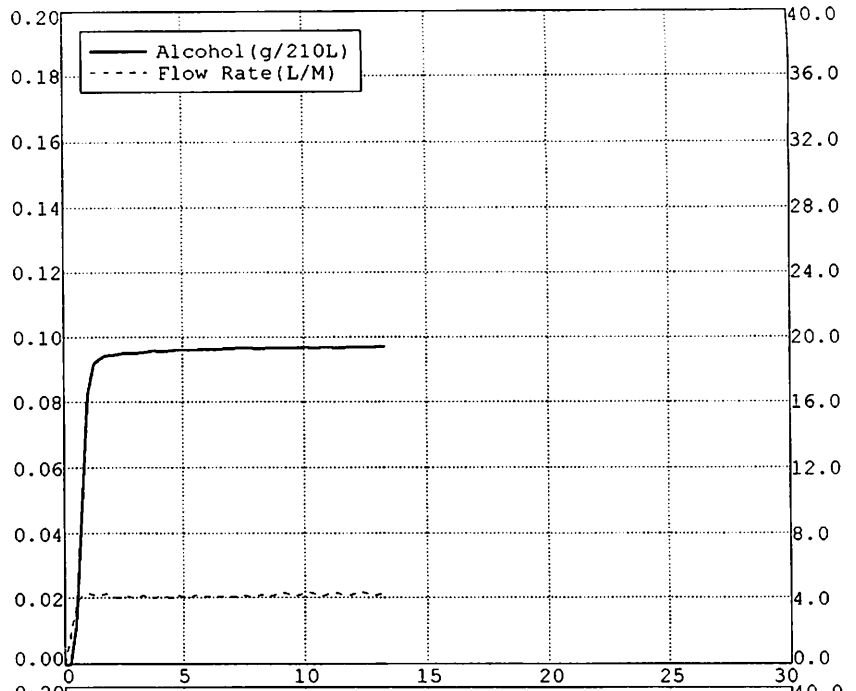

SOLUTION CHANGE

CFO
Latic




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 10/09/2019

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:20
INTERNAL STANDARD	VERIFIED	23:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:21
BLANK TEST	0.00	23:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:22
BLANK TEST	0.00	23:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:23
BLANK TEST	0.00	23:24

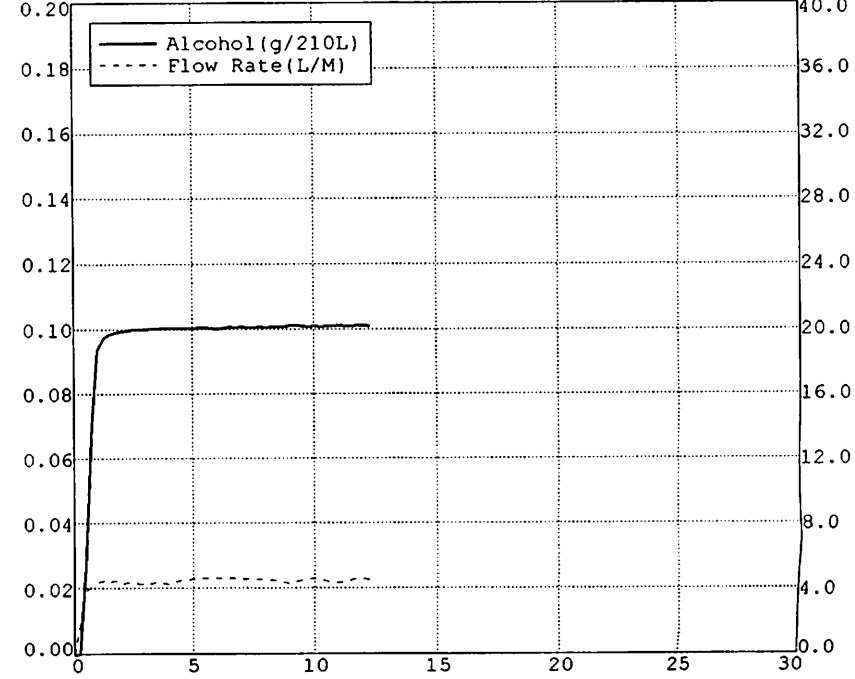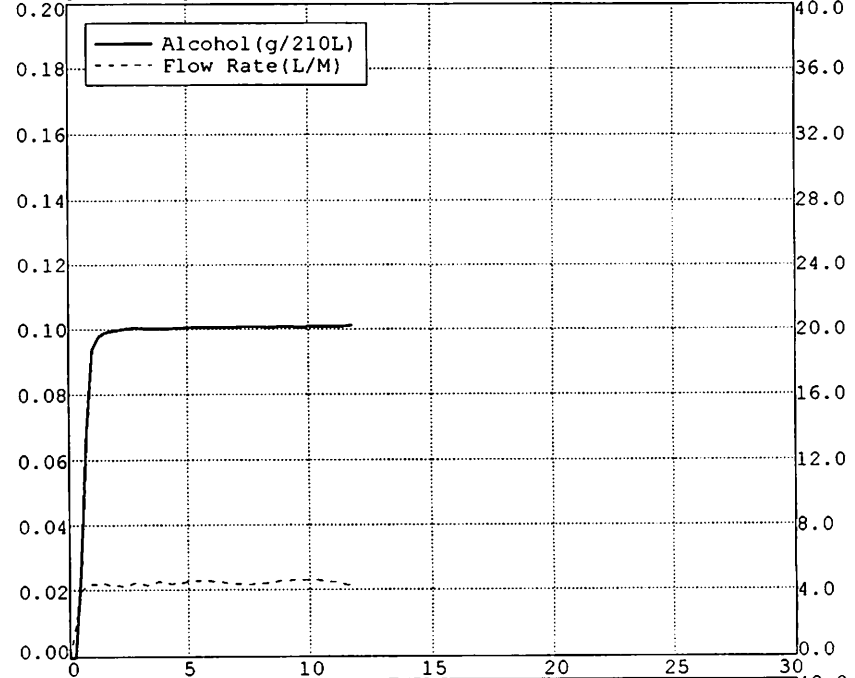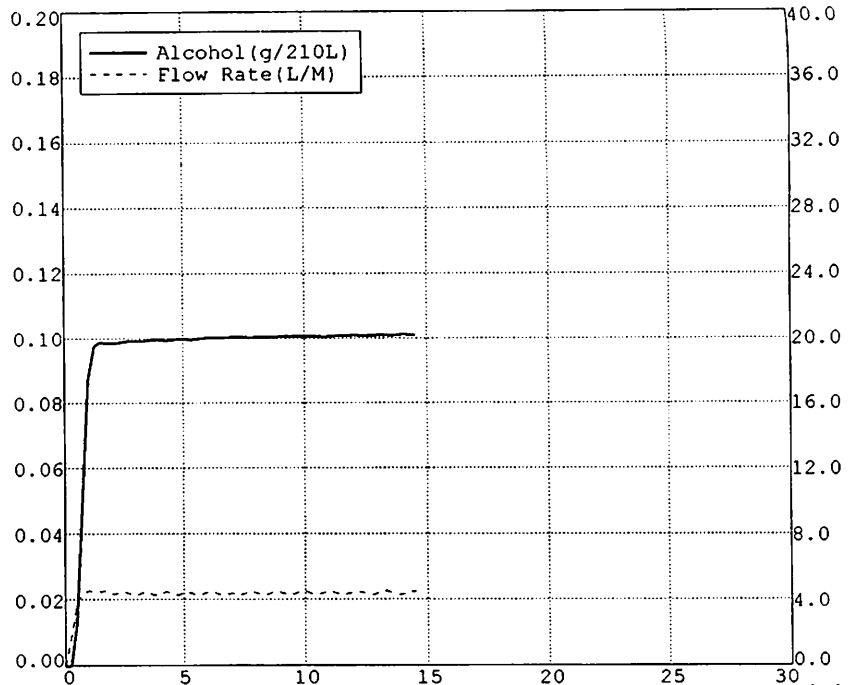

SUPERVISOR TEST

CFO

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 10/16/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:13
INTERNAL STANDARD	VERIFIED	20:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	20:14
BLANK TEST	0.00	20:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	20:15
BLANK TEST	0.00	20:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	20:16
BLANK TEST	0.00	20:17

