

SUPERVISOR TEST




ONEIDA CO.  
SHERIFF'S DEPT  
DATAMASTER dmt: 123906

Date: 04/02/2020

OPERATOR NAME:  
AARON P AVARD  
Permit #: 35561  
Operator Agency/Dept: ONEIDA CO. SO  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:52
INTERNAL STANDARD	VERIFIED	14:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:53
BLANK TEST	0.00	14:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:54
BLANK TEST	0.00	14:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:55
BLANK TEST	0.00	14:56

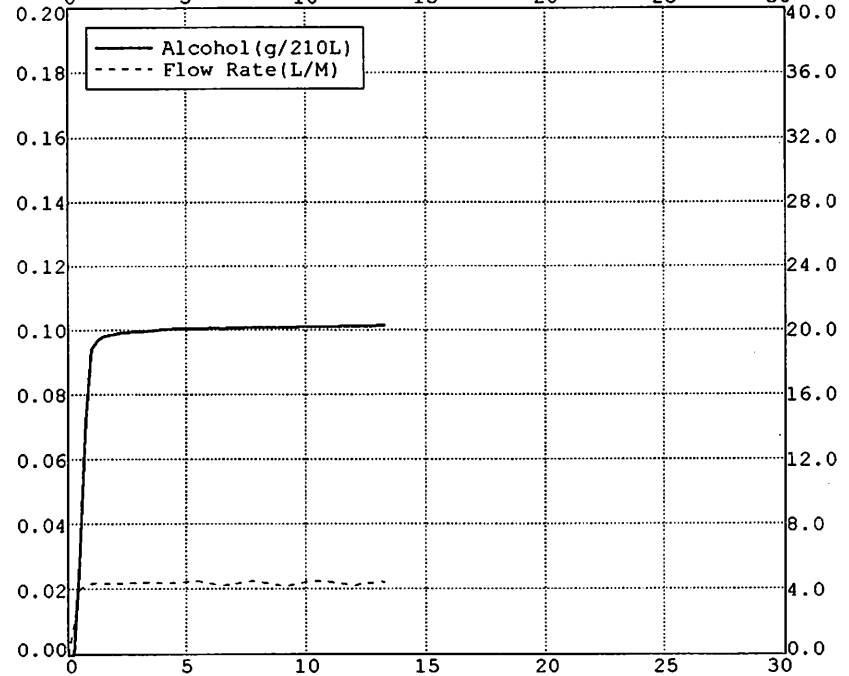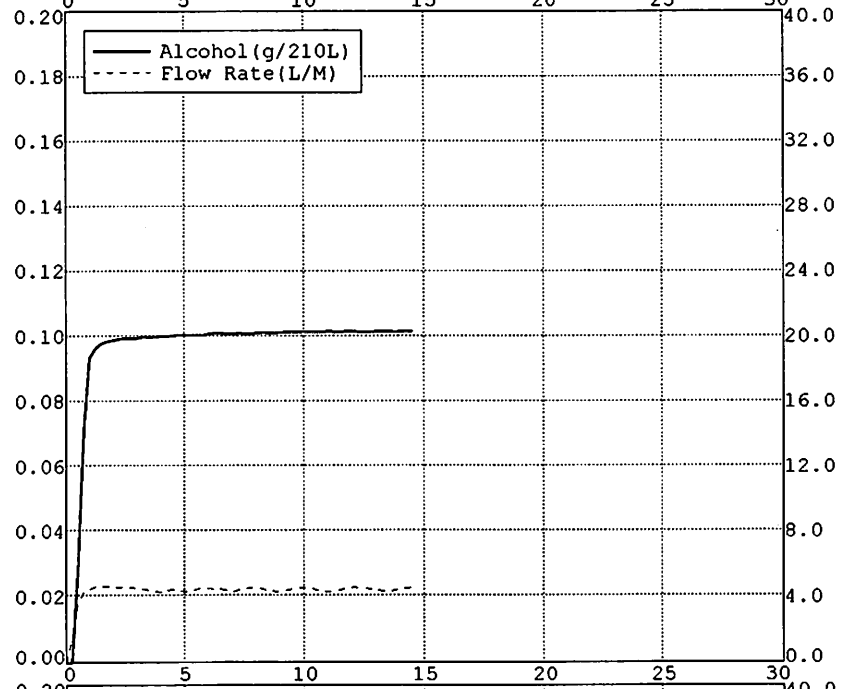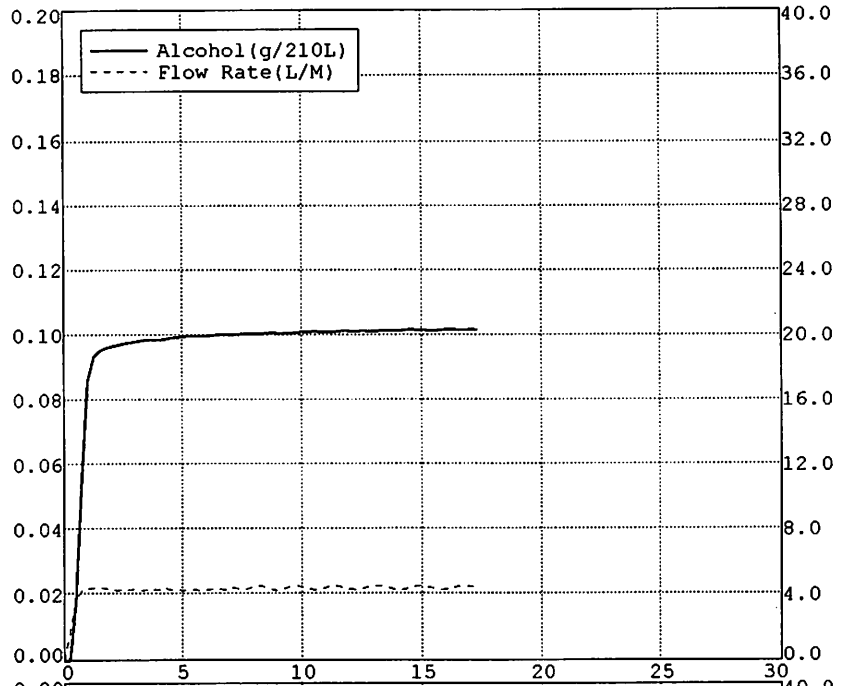

SUPERVISOR TEST

ONEIDA CO.  
SHERIFF'S DEPT  
DATAMASTER dmt: 123906

Date: 04/08/2020

OPERATOR NAME:  
BRANDON J RUTLEDGE  
Permit #: 43762  
Operator Agency/Dept: ONEIDA CO. SO  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:16
INTERNAL STANDARD	VERIFIED	22:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:16
BLANK TEST	0.00	22:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:17
BLANK TEST	0.00	22:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:19
BLANK TEST	0.00	22:19

*CFR*

