

SUPERVISOR TEST

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906



Date: 05/06/2020

OPERATOR NAME:
BRANDON J RUTLEDGE
Permit #: 43762
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:18
INTERNAL STANDARD	VERIFIED	21:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:19
BLANK TEST	0.00	21:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:20
BLANK TEST	0.00	21:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:21
BLANK TEST	0.00	21:22

CFO

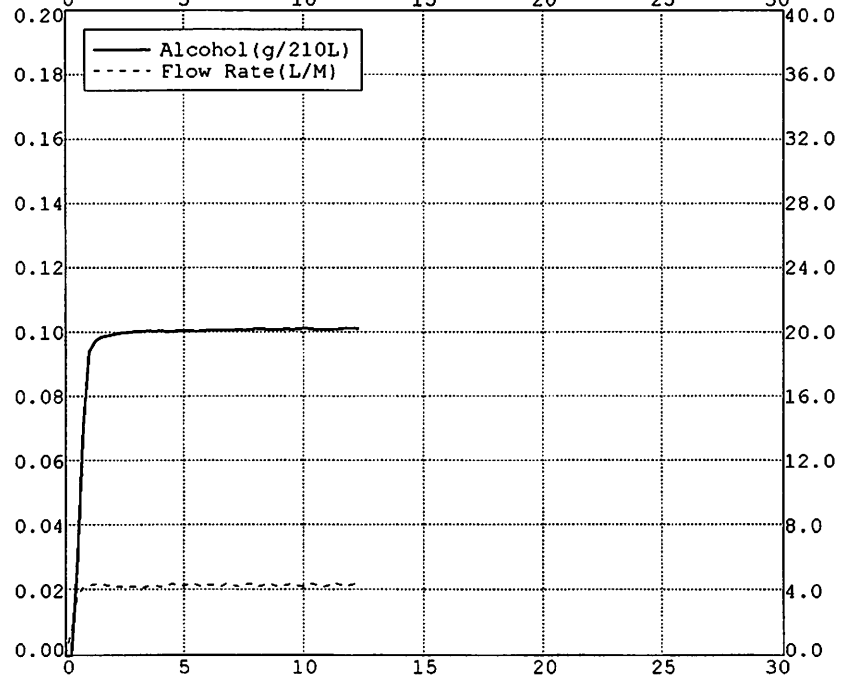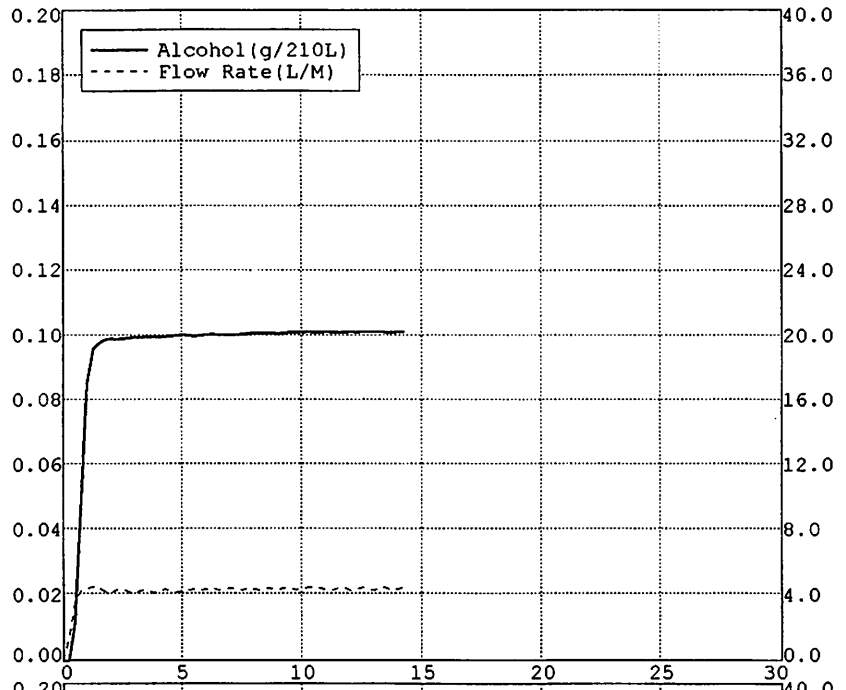

SUPERVISOR TEST

CFD

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 05/13/2020

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:55
INTERNAL STANDARD	VERIFIED	19:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:55
BLANK TEST	0.00	19:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:57
BLANK TEST	0.00	19:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:58
BLANK TEST	0.00	19:59

||-L>C@D♥@_o@@

