

SOLUTION CHANGE




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 02/01/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 19:26 |
| INTERNAL STANDARD | VERIFIED | 19:27 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 19:27 |
| BLANK TEST | 0.00 | 19:28 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 19:28 |
| BLANK TEST | 0.00 | 19:29 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 19:29 |
| BLANK TEST | 0.00 | 19:30 |

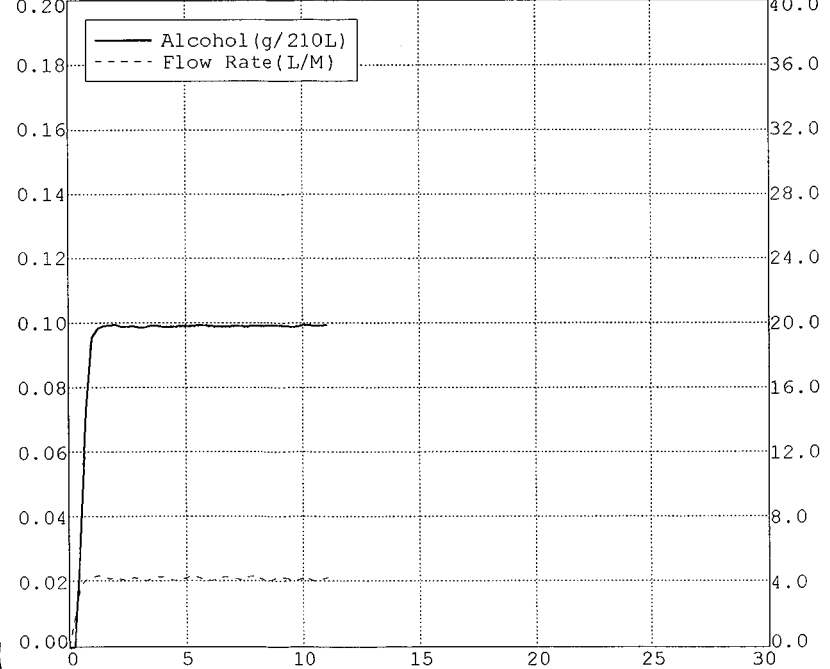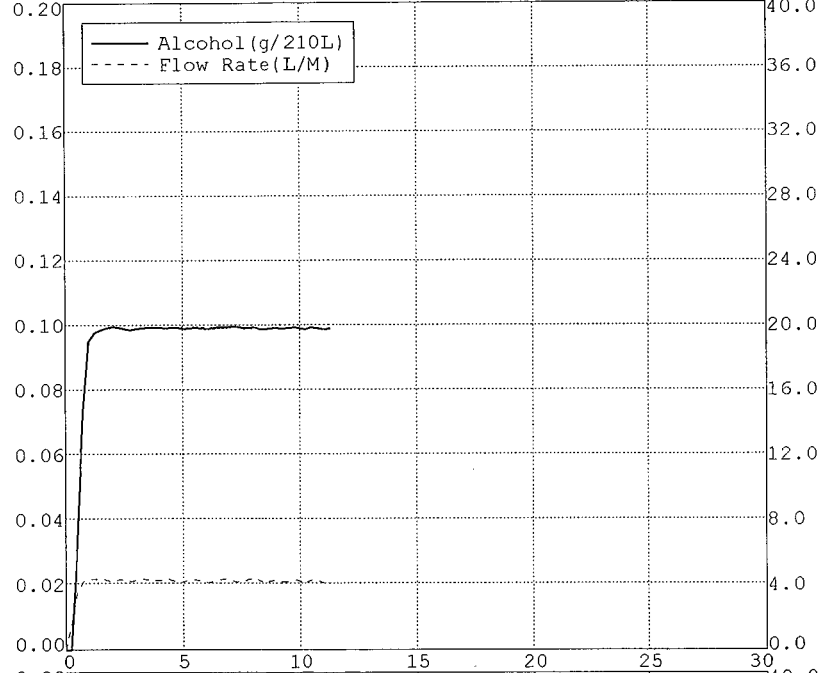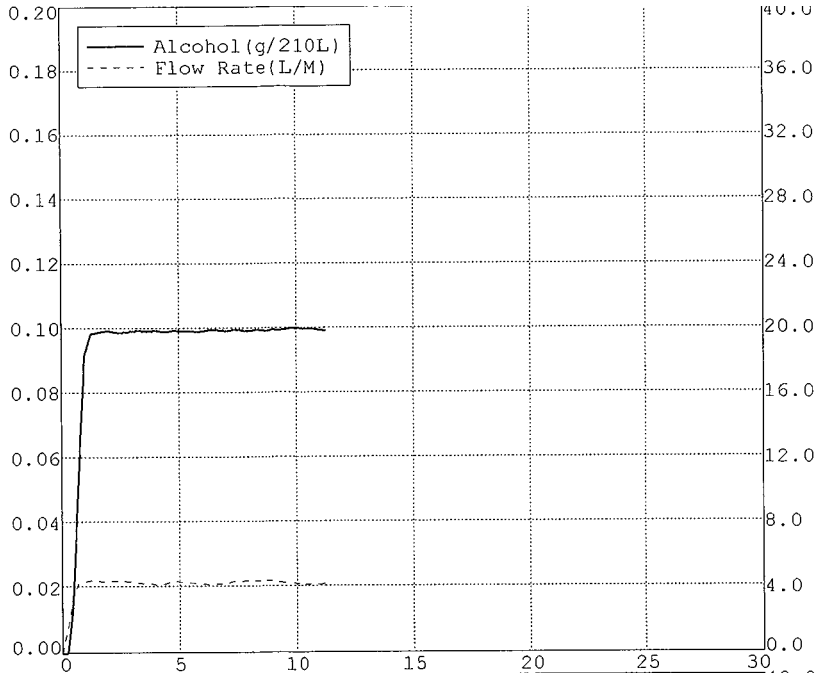

Hollie Kennedy Rome PD 02/01/19
1085

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 02/08/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 15:30 |
| INTERNAL STANDARD | VERIFIED | 15:30 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 15:31 |
| BLANK TEST | 0.00 | 15:32 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 15:32 |
| BLANK TEST | 0.00 | 15:33 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 15:33 |
| BLANK TEST | 0.00 | 15:34 |

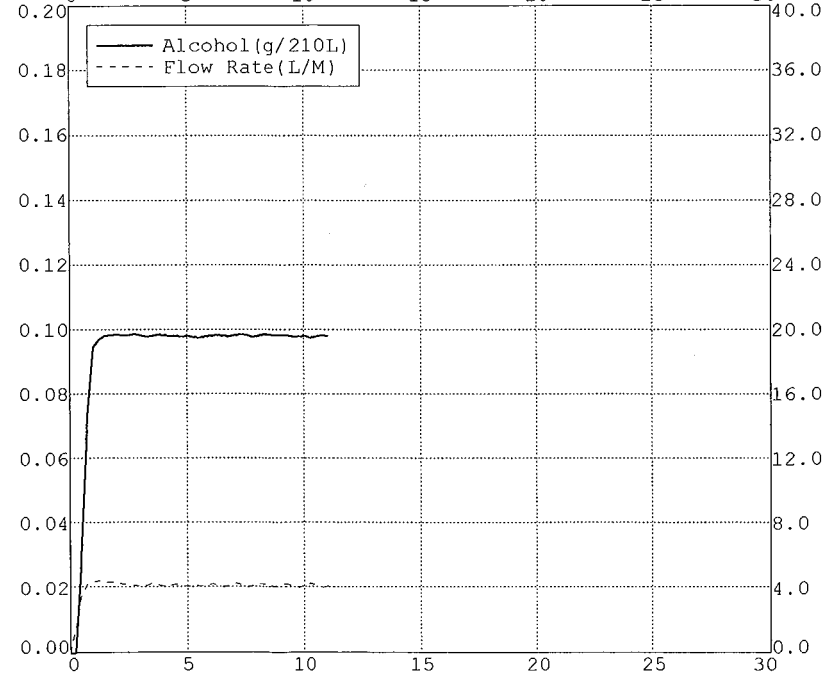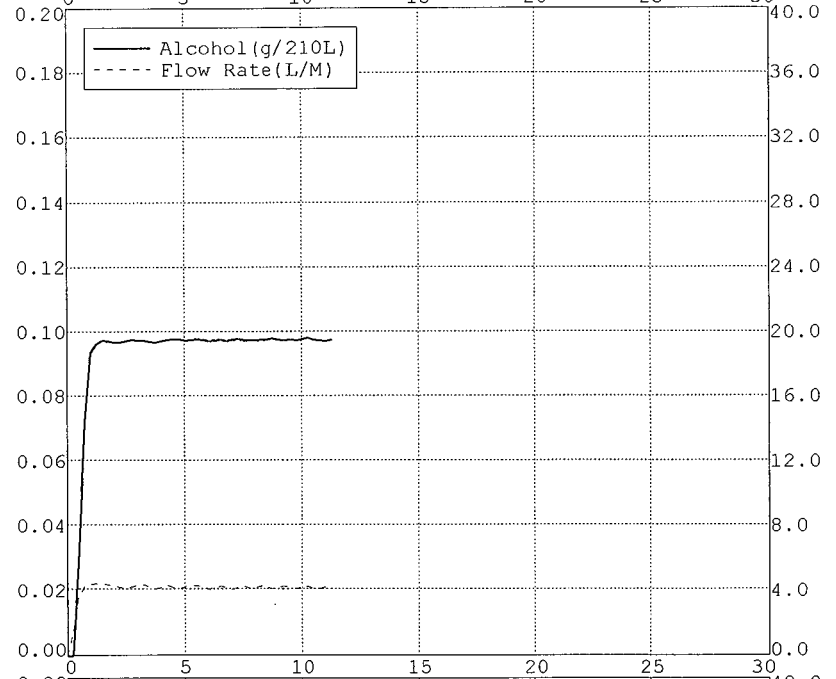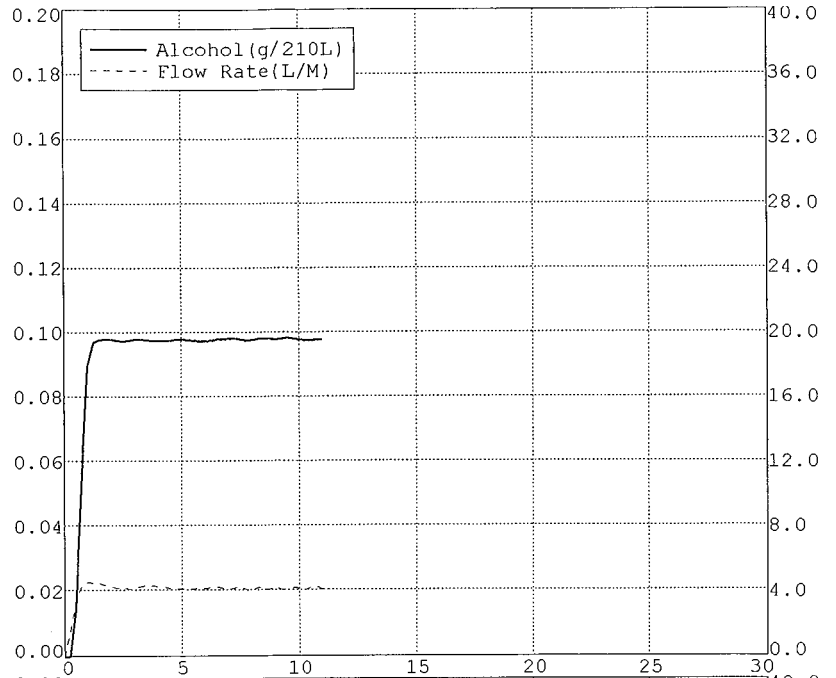

Hollie B Kennedy Rome PD 02/08/19
Reference Standard 18360

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 02/15/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 22:33 |
| INTERNAL STANDARD | VERIFIED | 22:33 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 22:34 |
| BLANK TEST | 0.00 | 22:35 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 22:35 |
| BLANK TEST | 0.00 | 22:36 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 22:36 |
| BLANK TEST | 0.00 | 22:37 |

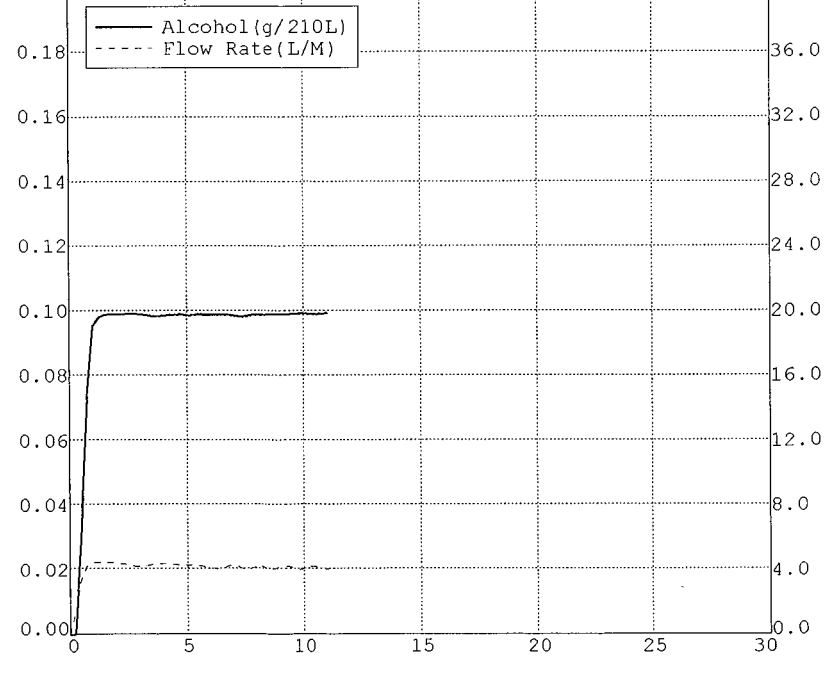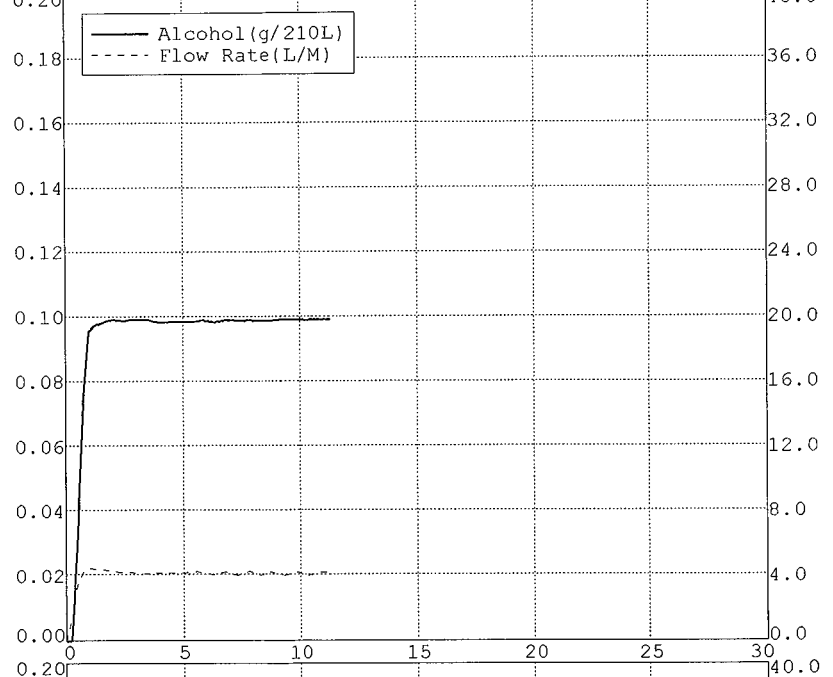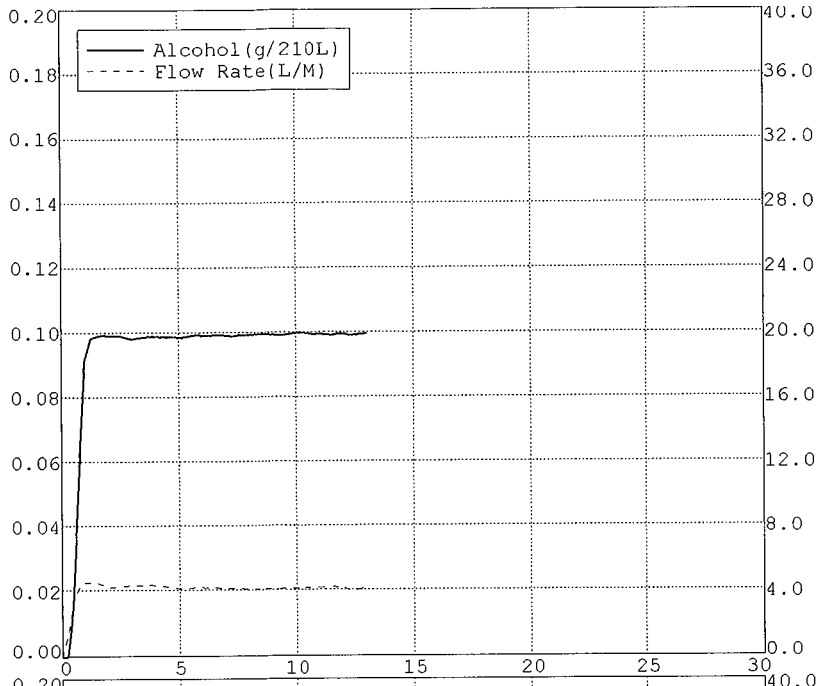

Hollie Kennedy Rome PD 02/15/19
Rome PD

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 02/22/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 19:10 |
| INTERNAL STANDARD | VERIFIED | 19:10 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 19:10 |
| BLANK TEST | 0.00 | 19:11 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 19:11 |
| BLANK TEST | 0.00 | 19:12 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 19:13 |
| BLANK TEST | 0.00 | 19:13 |

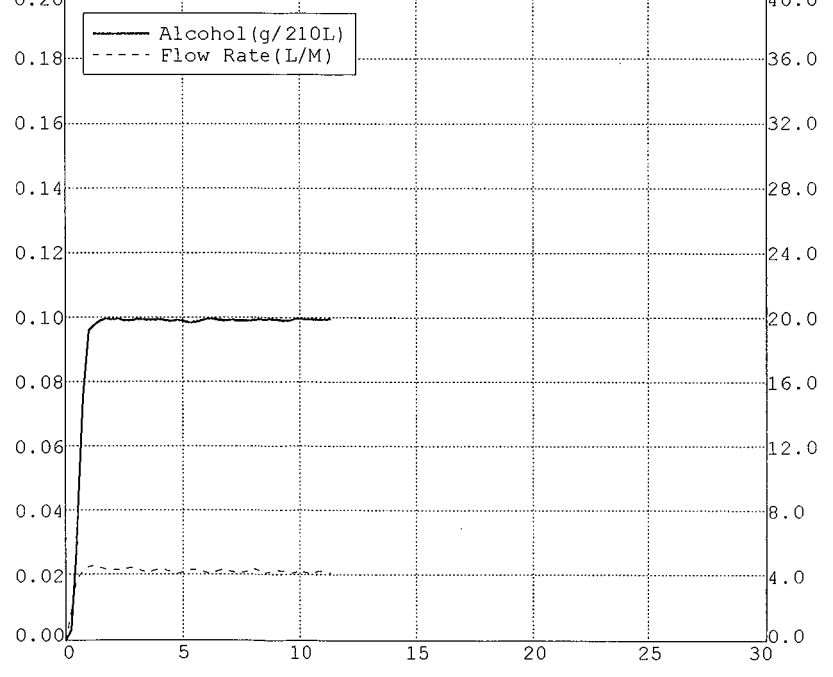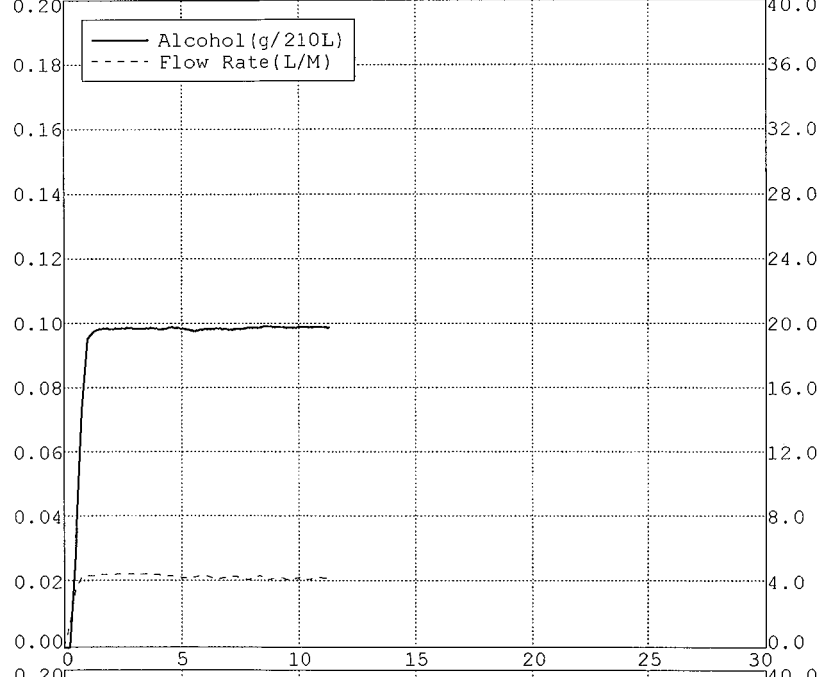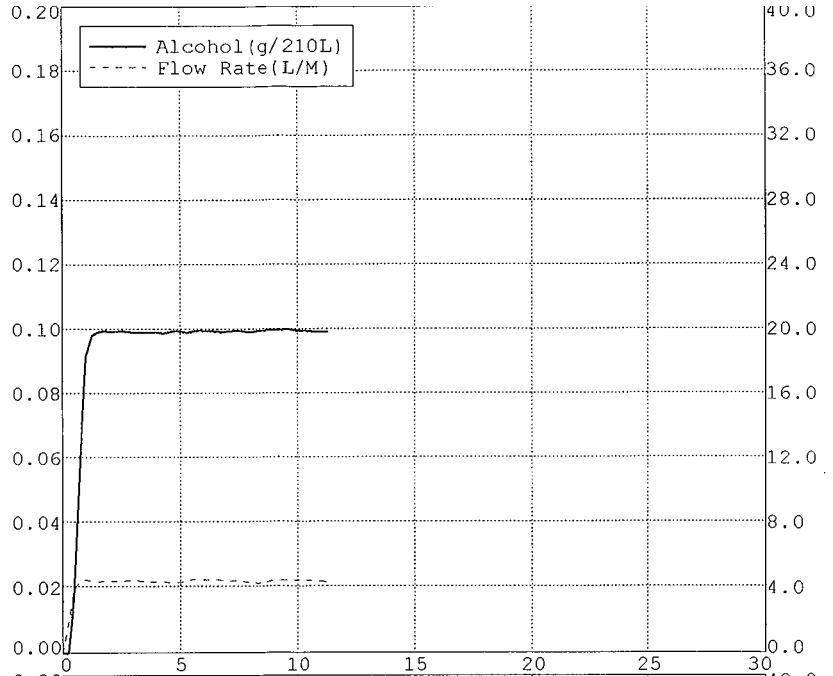

Hollie Kennedy Rome PD 02/22/19
Alm 1005