

SUPERVISOR TEST




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 01/17/2020

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:23
INTERNAL STANDARD	VERIFIED	15:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:24
BLANK TEST	0.00	15:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:25
BLANK TEST	0.00	15:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:26
BLANK TEST	0.00	15:27

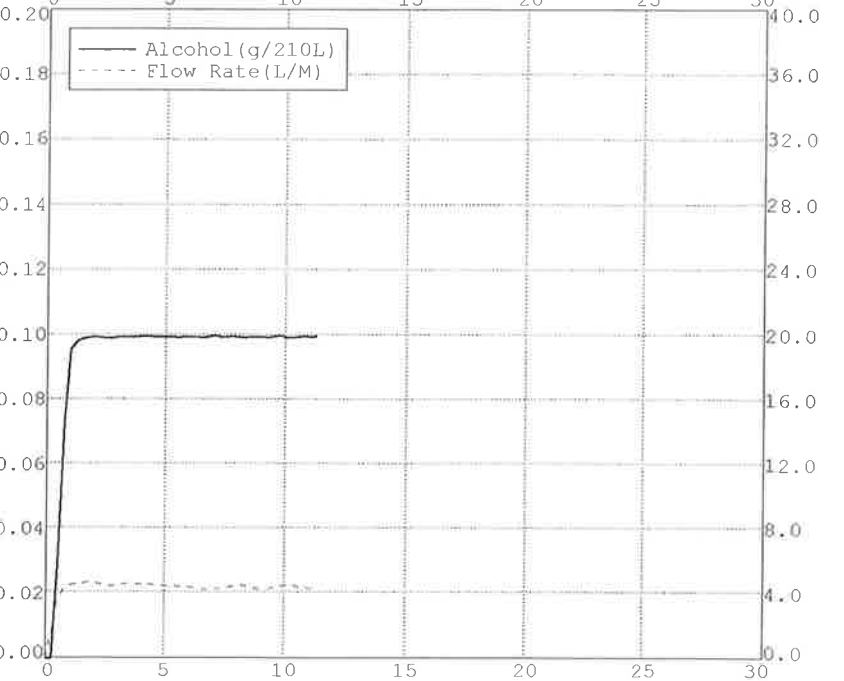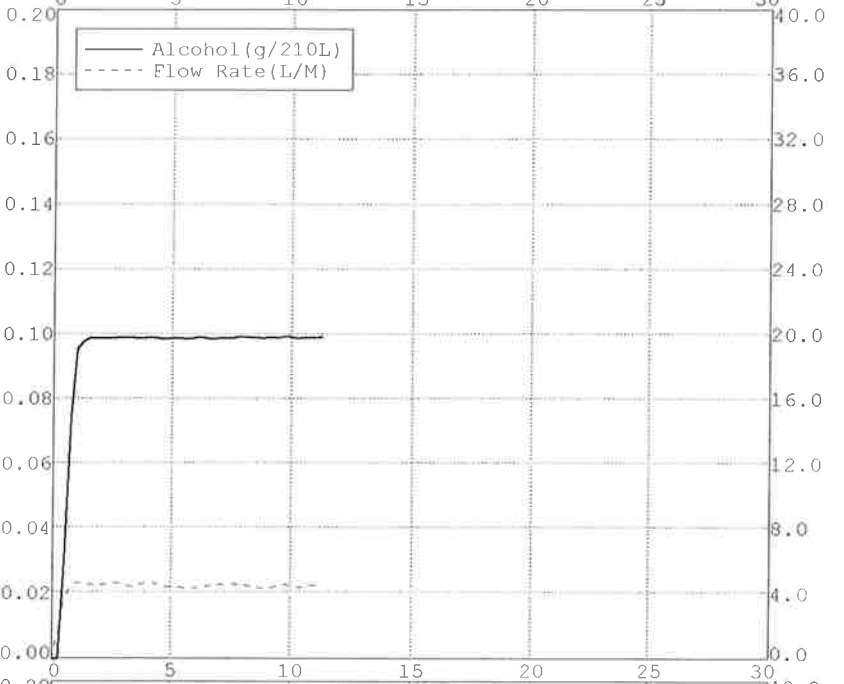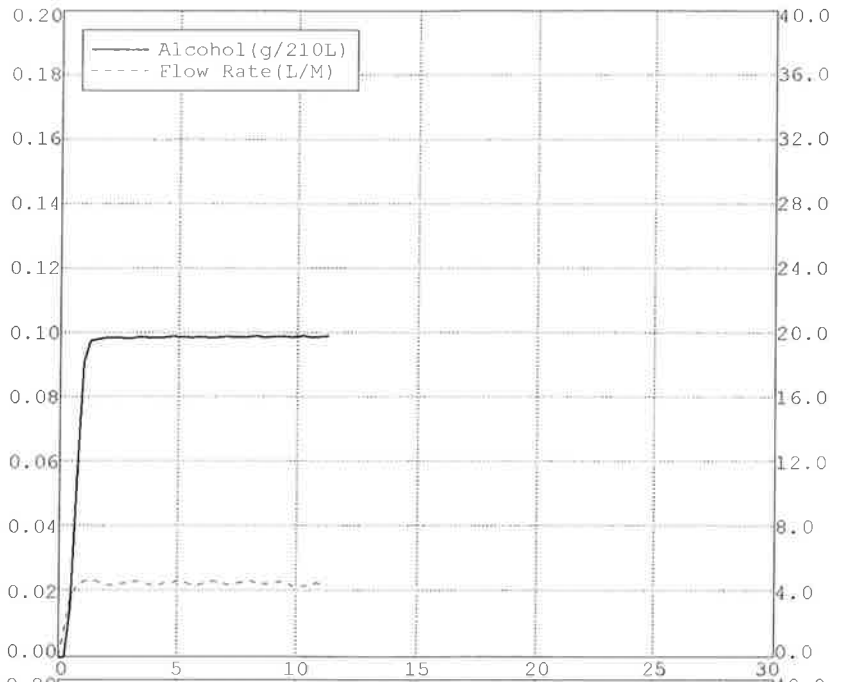

*Hollie B. Silverman 01/17/2020 Rome PD*  
*10805*