

SUPERVISOR TEST


ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 02/21/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:30
INTERNAL STANDARD	VERIFIED	19:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:31
BLANK TEST	0.00	19:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:32
BLANK TEST	0.00	19:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:33
BLANK TEST	0.00	19:34

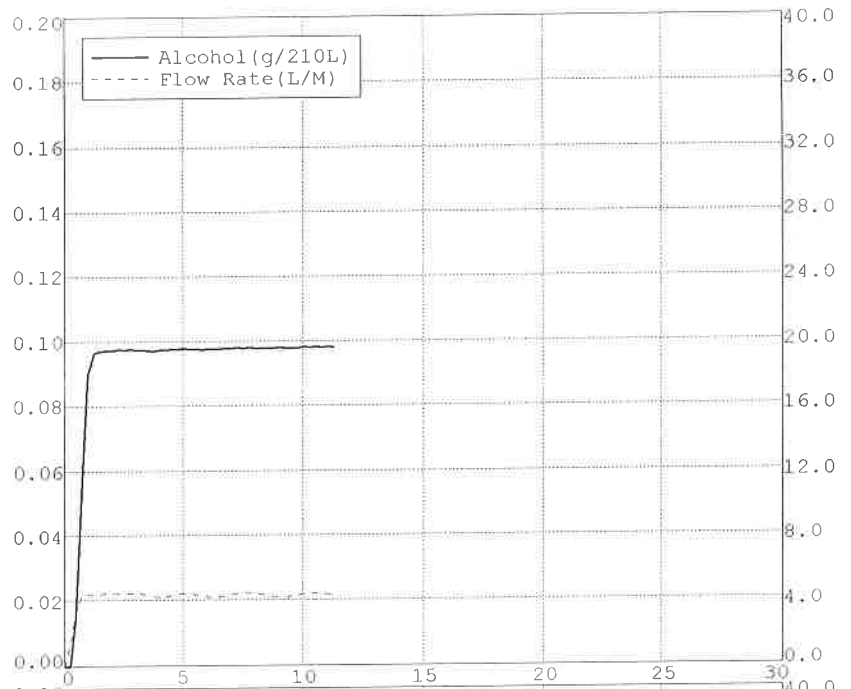

Hollie B. Silverman Rome PD 02/21/2020
Hollie B. Silverman