

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 03/20/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:43
INTERNAL STANDARD	VERIFIED	07:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:44
BLANK TEST	0.00	07:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:45
BLANK TEST	0.00	07:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:46
BLANK TEST	0.00	07:47

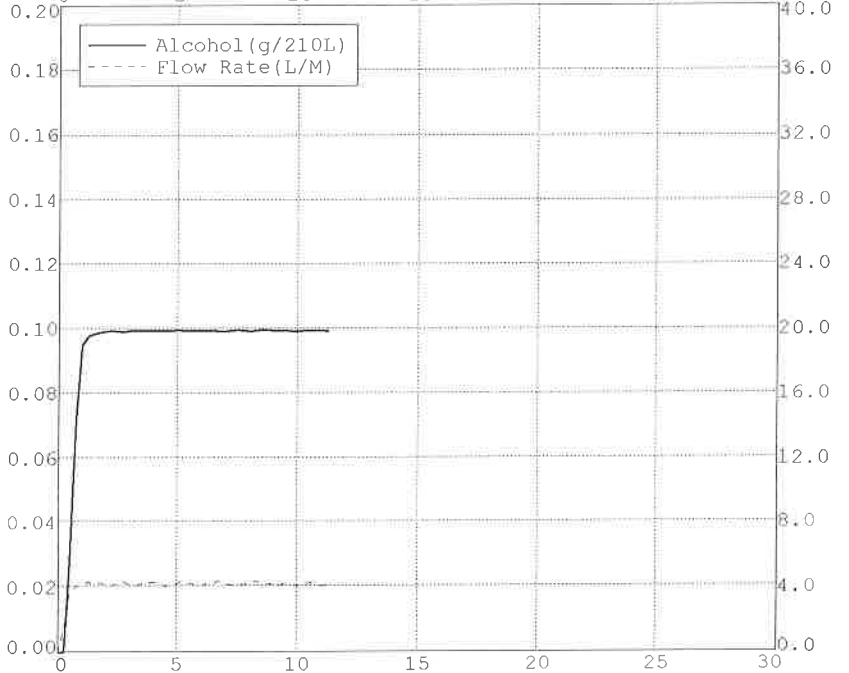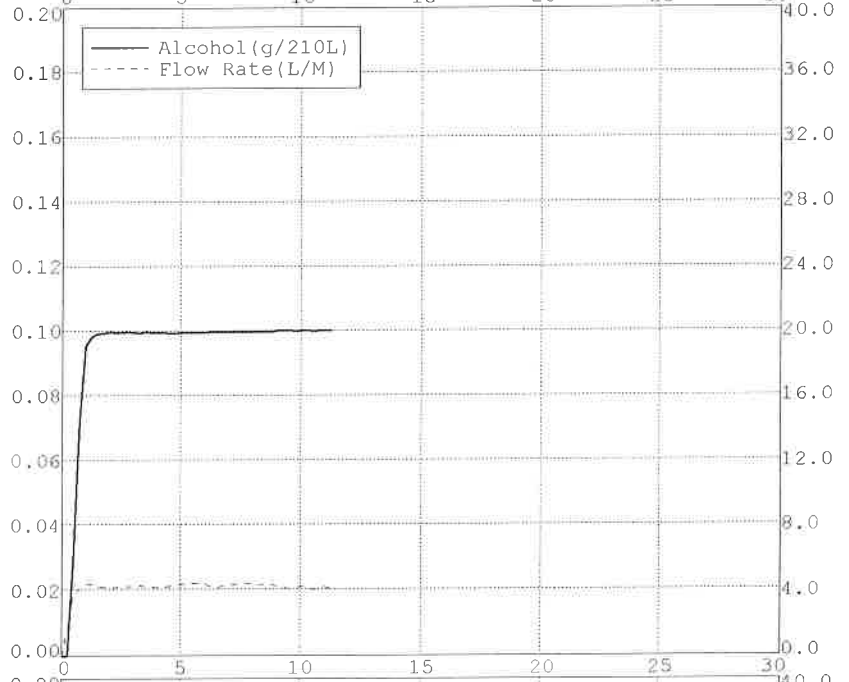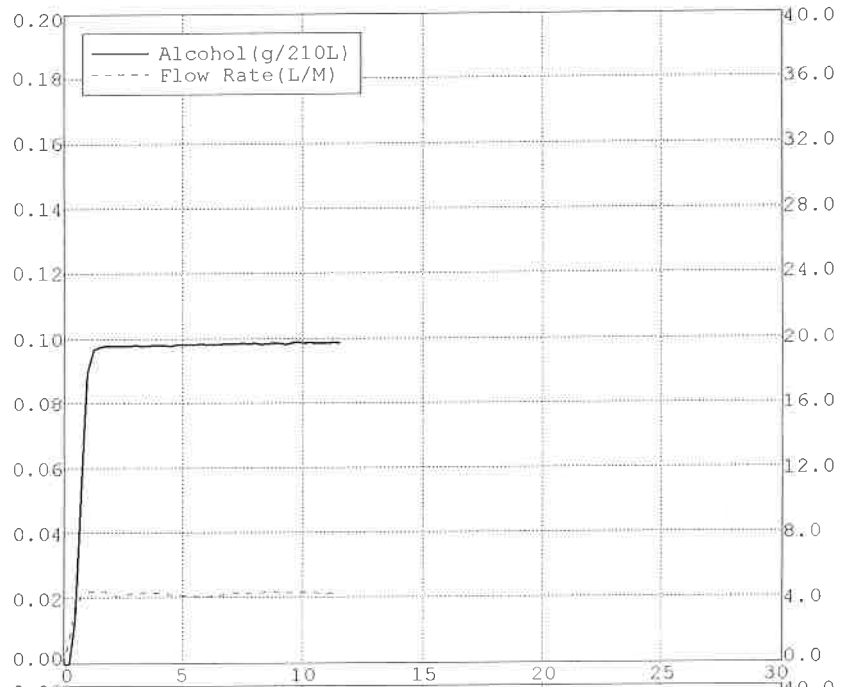

Hollie B Silverman Rome B 03/20/2020
Hollie B Silverman 10805