

SUPERVISOR TEST



ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 04/17/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:38
INTERNAL STANDARD	VERIFIED	16:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:38
BLANK TEST	0.00	16:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:39
BLANK TEST	0.00	16:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:41
BLANK TEST	0.00	16:41

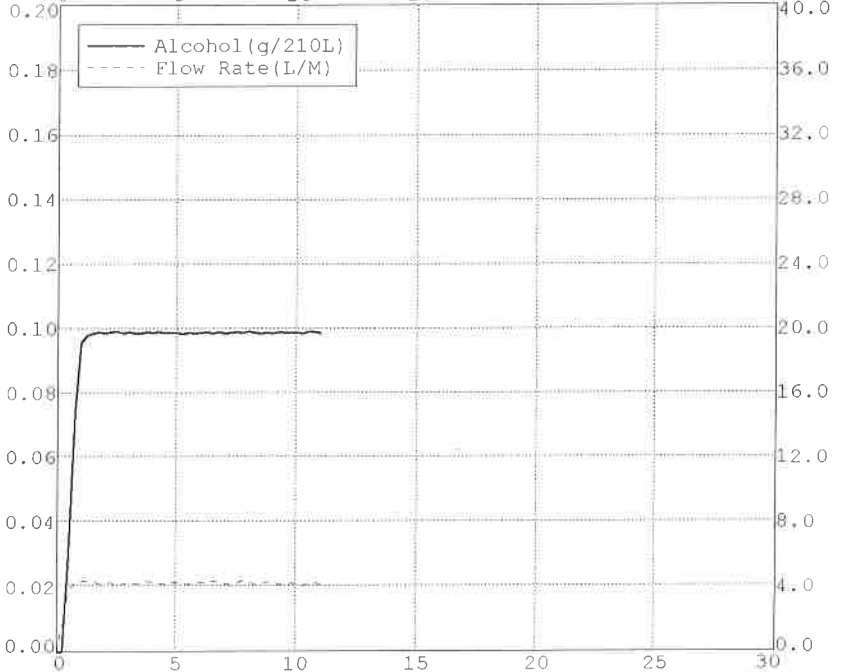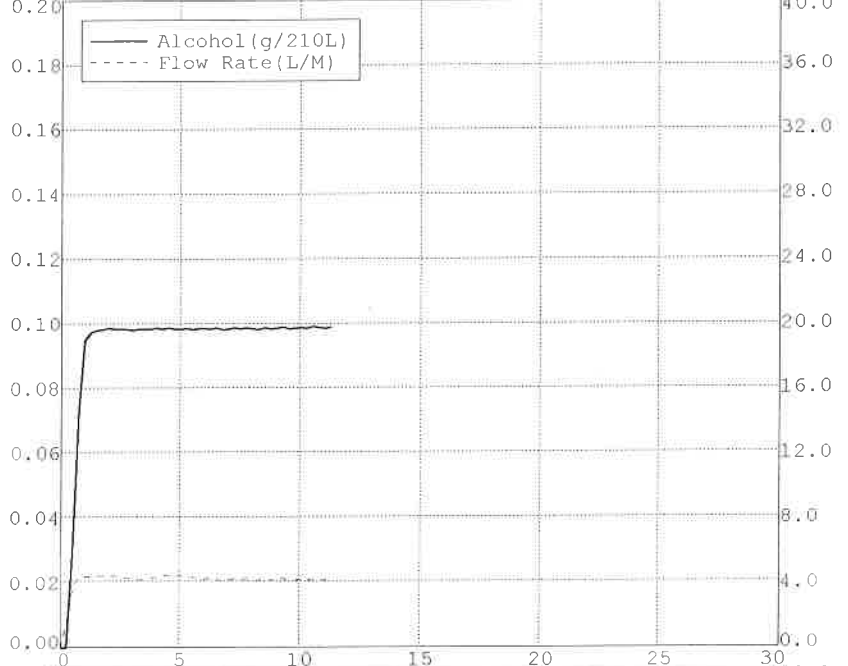

Hollie B Silverman Rome PD 04/17/2020
Hollie B Silverman 10/01