

SUPERVISOR TEST


ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 04/24/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:57
INTERNAL STANDARD	VERIFIED	19:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:58
BLANK TEST	0.00	19:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:59
BLANK TEST	0.00	20:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:00
BLANK TEST	0.00	20:01

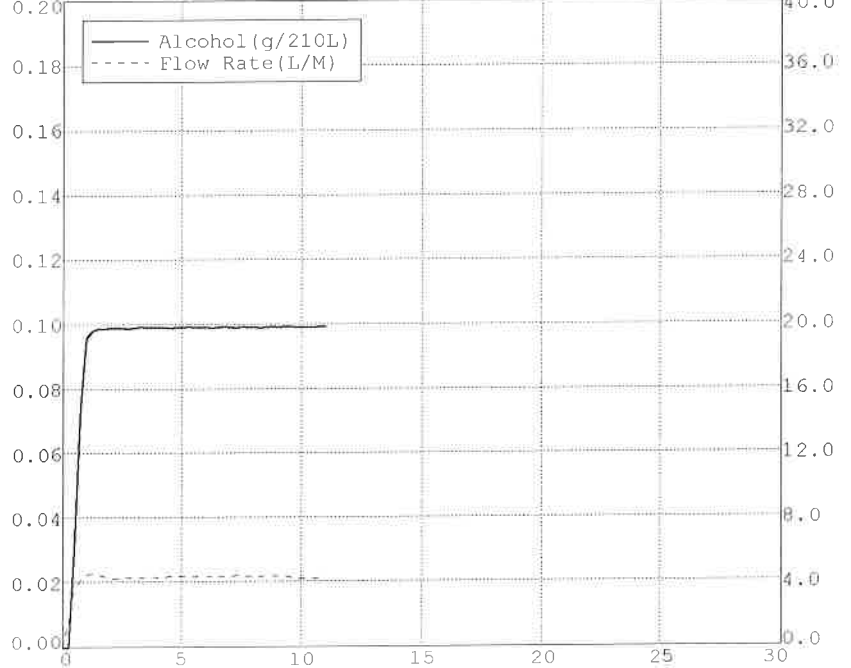

Hollie B. Silverman Rome PD 04/24/2020

Hollie B. Silverman 10105