

SUPERVISOR TEST




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 05/01/2020

OPERATOR NAME:
 HOLLIE B SILVERMAN
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:28
INTERNAL STANDARD	VERIFIED	16:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:28
BLANK TEST	0.00	16:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:30
BLANK TEST	0.00	16:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:31
BLANK TEST	0.00	16:32

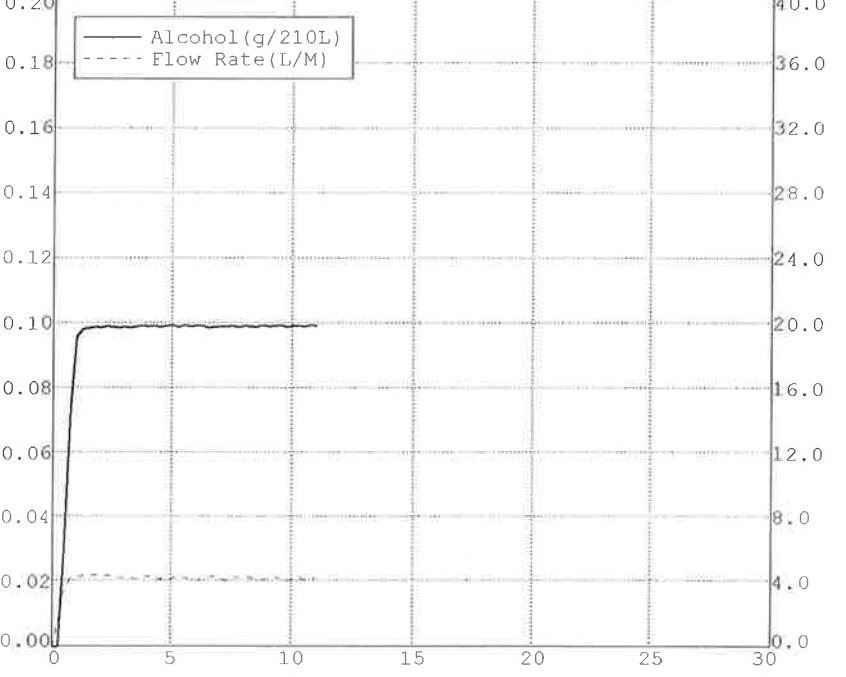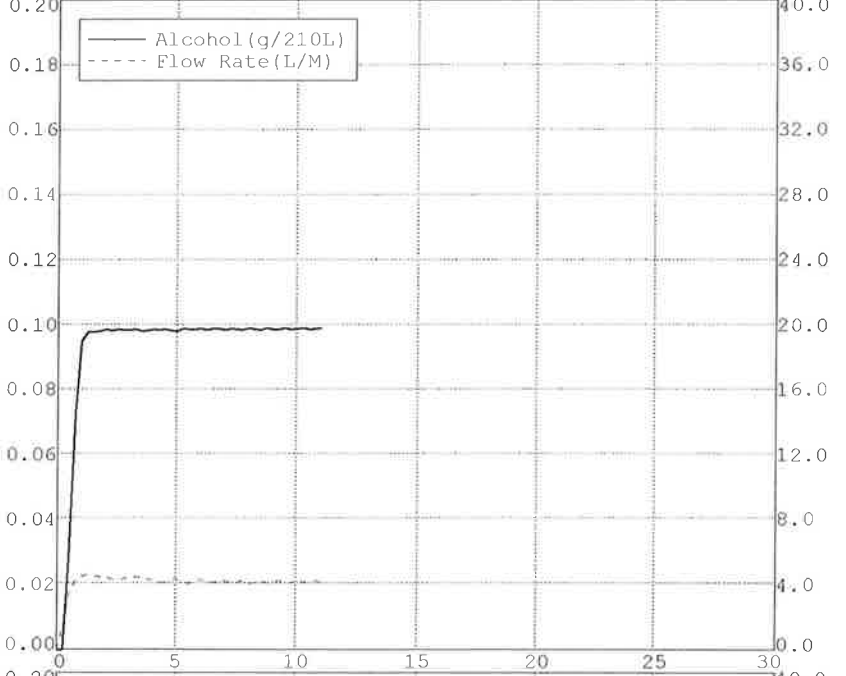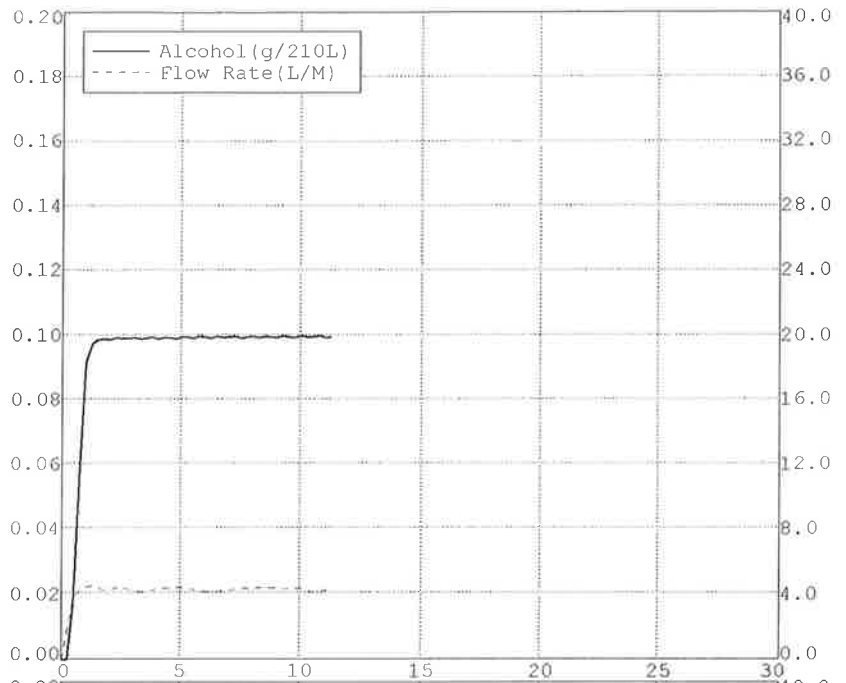

Hollie B. Silverman Rome PD 05/01/2020
 Hollie B. Silverman 10905