

SUPERVISOR TEST



ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 05/15/2020

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:52
INTERNAL STANDARD	VERIFIED	19:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:53
BLANK TEST	0.00	19:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:54
BLANK TEST	0.00	19:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:55
BLANK TEST	0.00	19:56

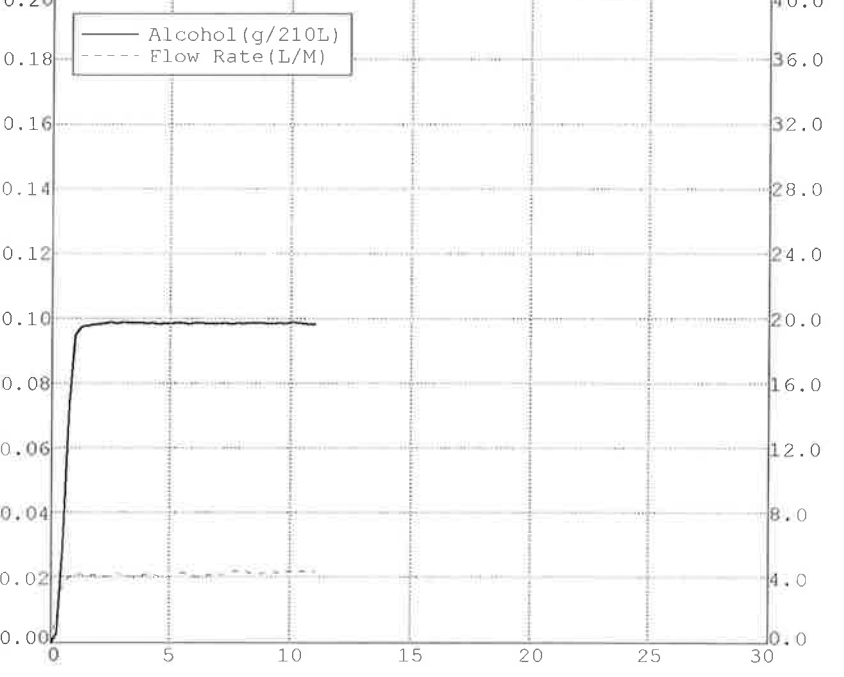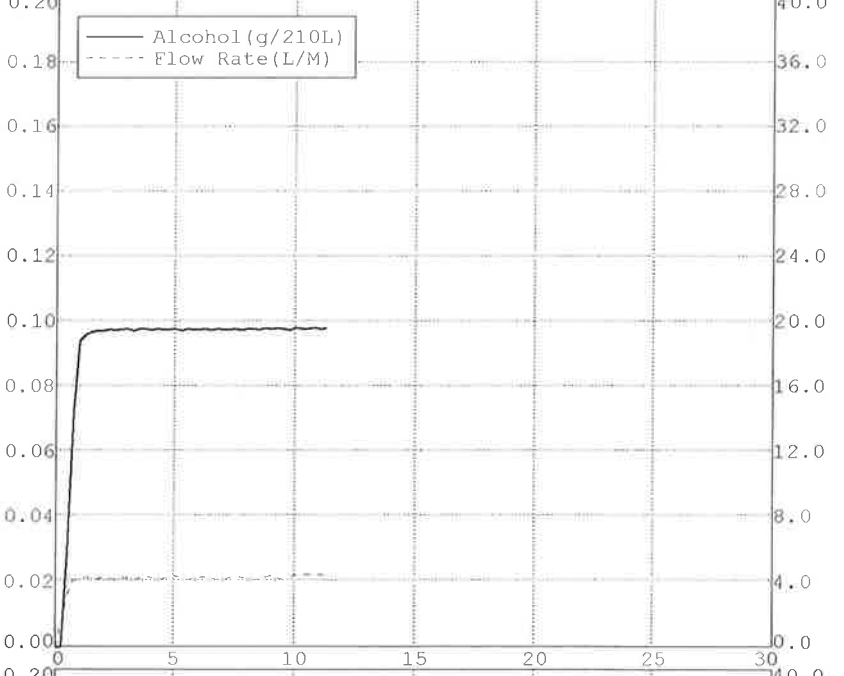

*Hollie B Silverman Rome PD 05/15/20*  
*Hollie B Silverman 1095*

SUPERVISOR TEST

ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106


Date: 05/15/2020

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:42
INTERNAL STANDARD	VERIFIED	19:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:42

RFI Detected

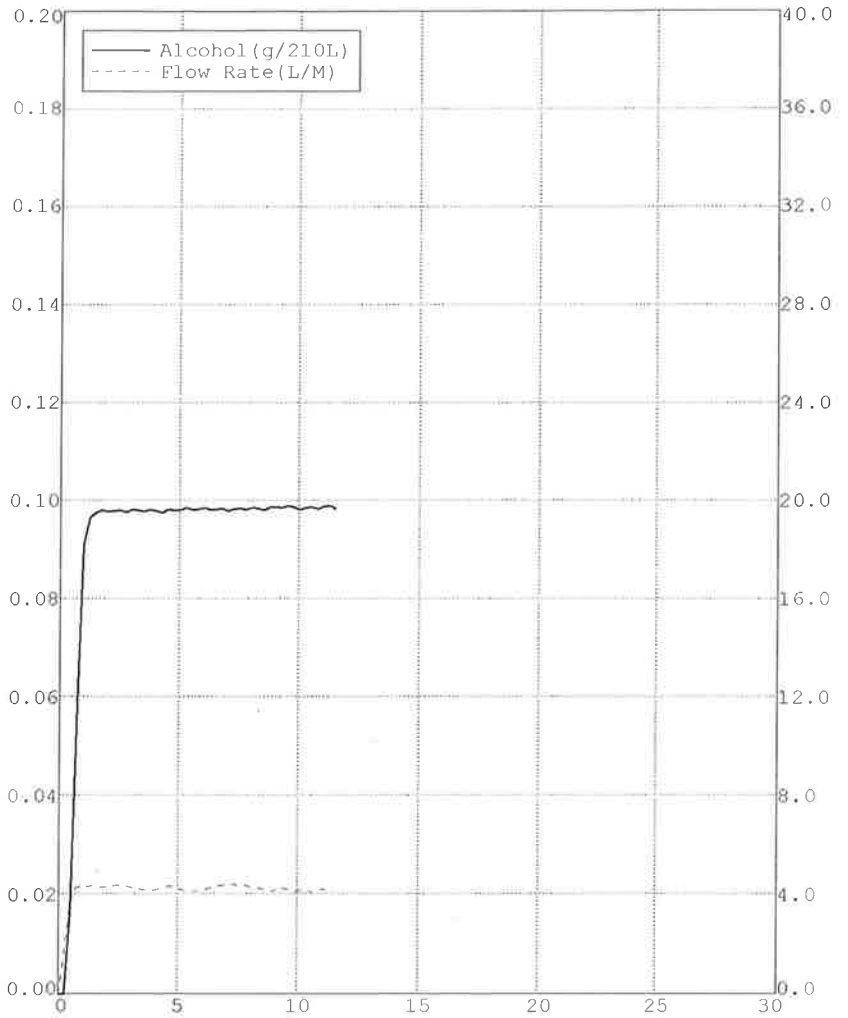

Hollie B Silverman Rome PD 05/15/2020  
Hollie B Silverman 10705