

SUPERVISOR TEST




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 05/22/2020

OPERATOR NAME:
 HOLLIE B SILVERMAN
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:05
INTERNAL STANDARD	VERIFIED	03:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:05
BLANK TEST	0.00	03:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:07
BLANK TEST	0.00	03:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:08
BLANK TEST	0.00	03:09

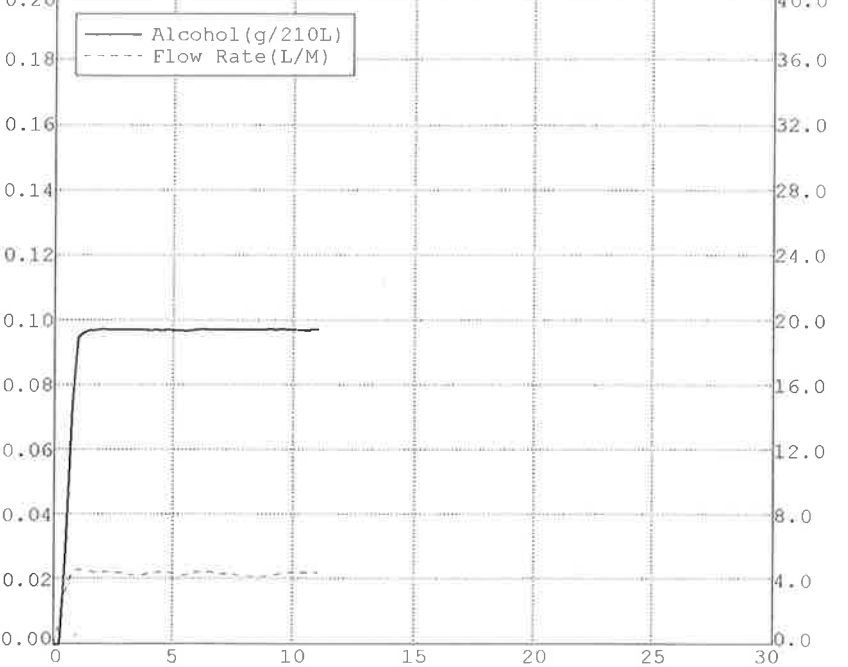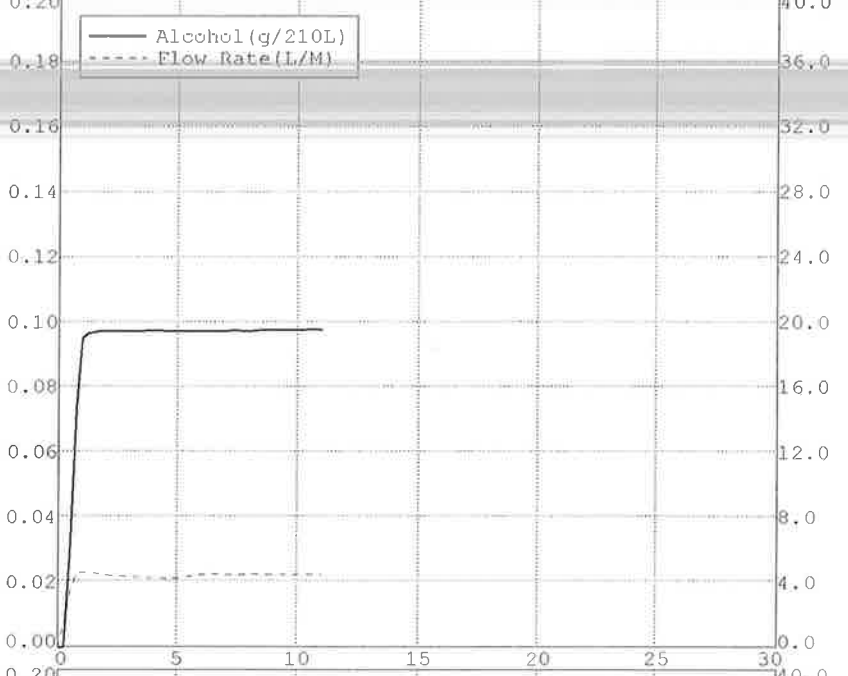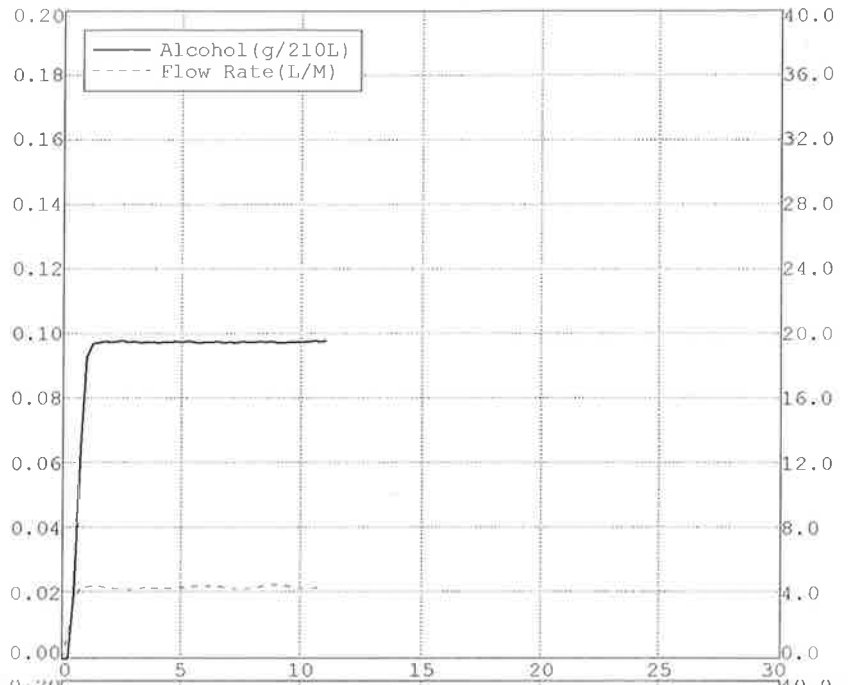

Hollie B. Silverman Rome PD 05/22/2020
 Hollie B. Silverman 0805