

SUPERVISOR TEST




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 05/29/2020

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:27
INTERNAL STANDARD	VERIFIED	15:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:27
BLANK TEST	0.00	15:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:28
BLANK TEST	0.00	15:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:29
BLANK TEST	0.00	15:30

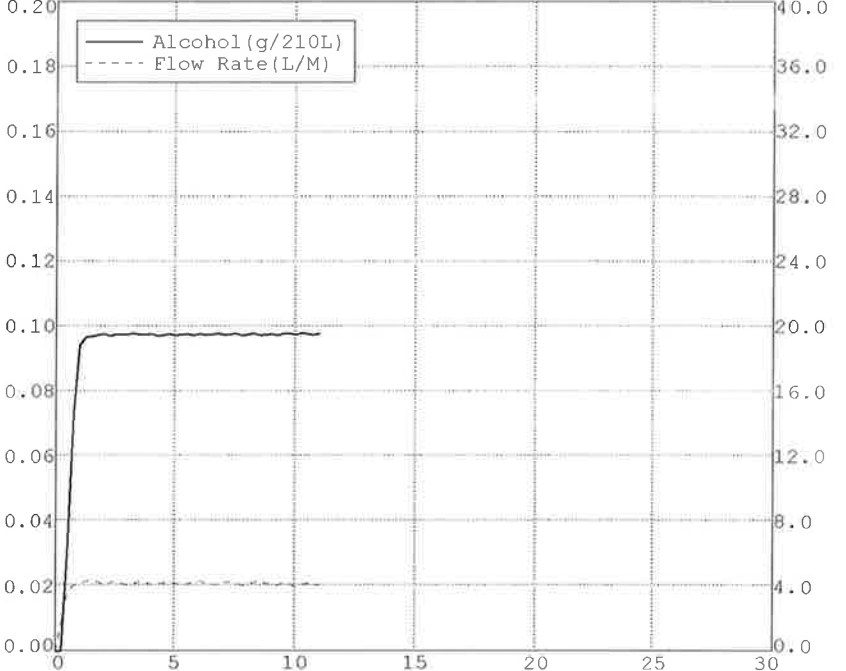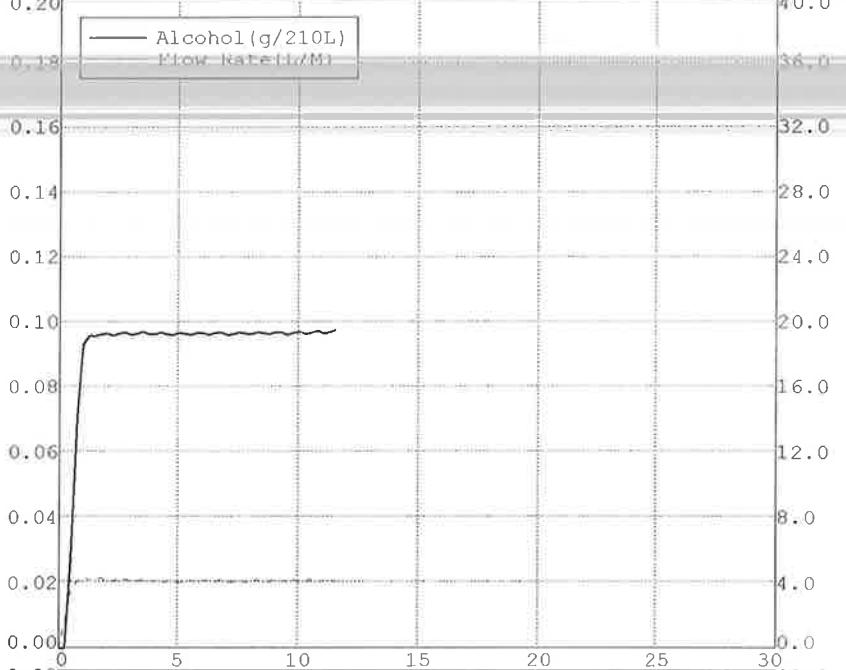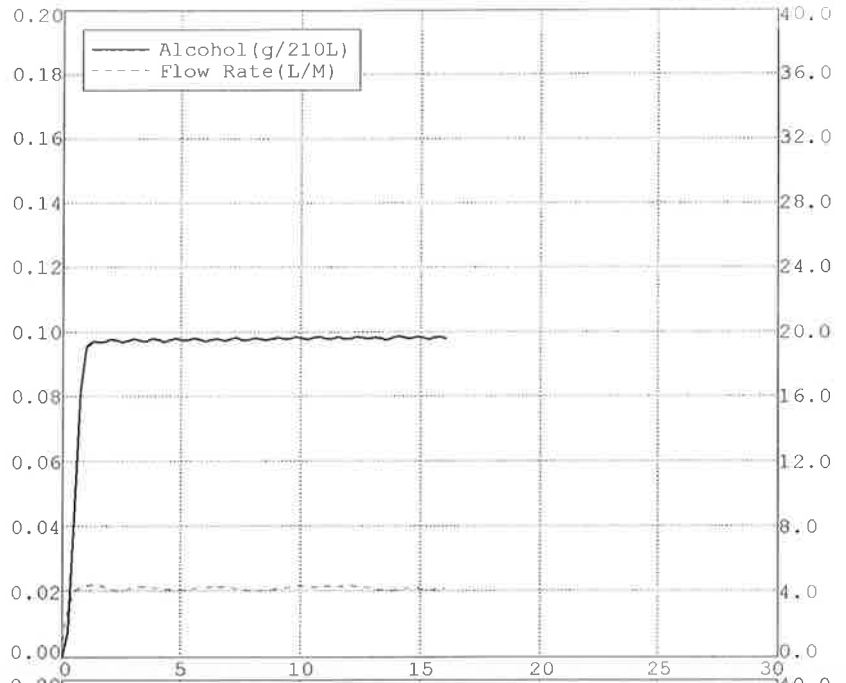

Hollie B. Silverman Rome PD 05/29/2020  
Hollie B. Silverman 10908