

SOLUTION CHANGE

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 100282




Date: 04/02/2020

*RMJ*  
*20-10891*

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:20
INTERNAL STANDARD	VERIFIED	13:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	13:20
BLANK TEST	0.00	13:21
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	13:21
BLANK TEST	0.00	13:22
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	13:22
BLANK TEST	0.00	13:23

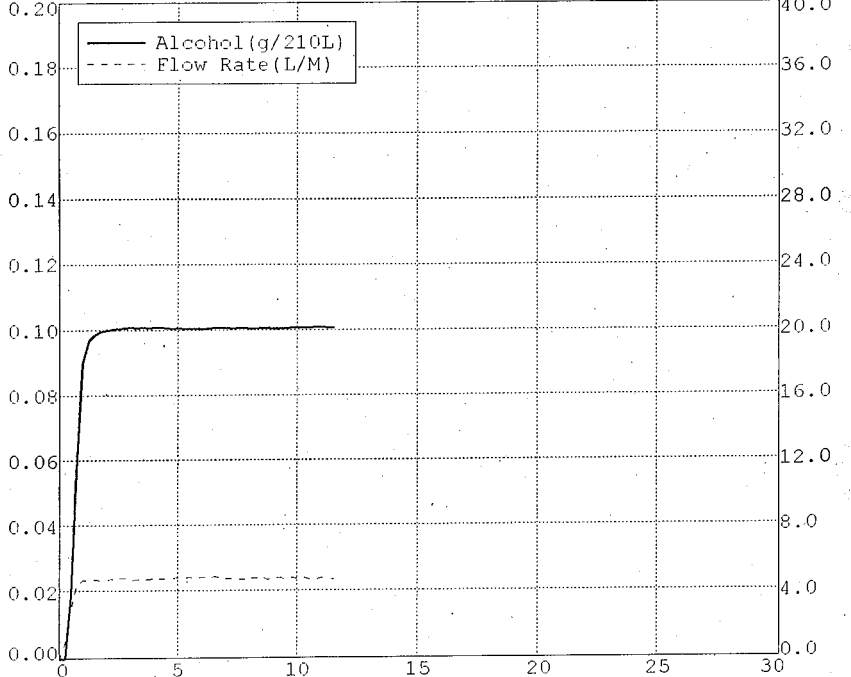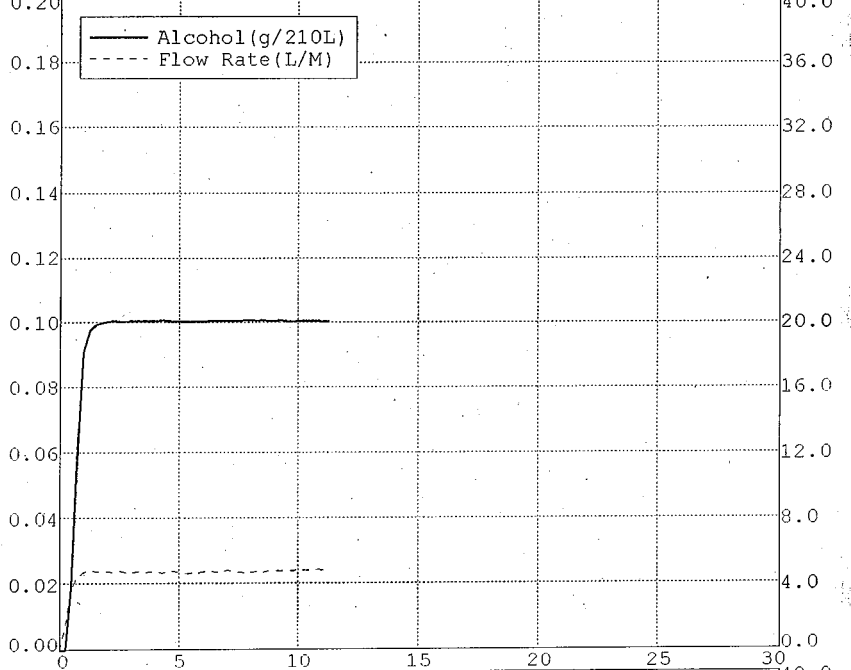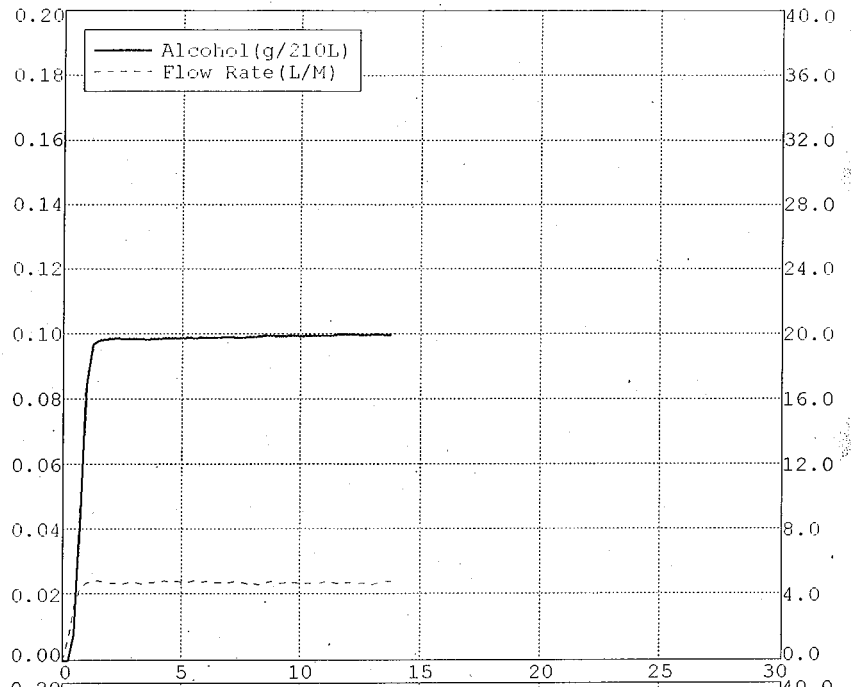

SOLUTION CHANGE

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 107308

Date: 04/02/2020

*2ms*  
*20-10841*

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:46
INTERNAL STANDARD	VERIFIED	13:46
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:47
BLANK TEST	0.00	13:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:48
BLANK TEST	0.00	13:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:49
BLANK TEST	0.00	13:50

