

SOLUTION CHANGE

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 02/03/2020

RMS
20-3734

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:29
INTERNAL STANDARD	VERIFIED	12:29
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:30
BLANK TEST	0.00	12:31
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:31
BLANK TEST	0.00	12:32
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:32
BLANK TEST	0.00	12:33

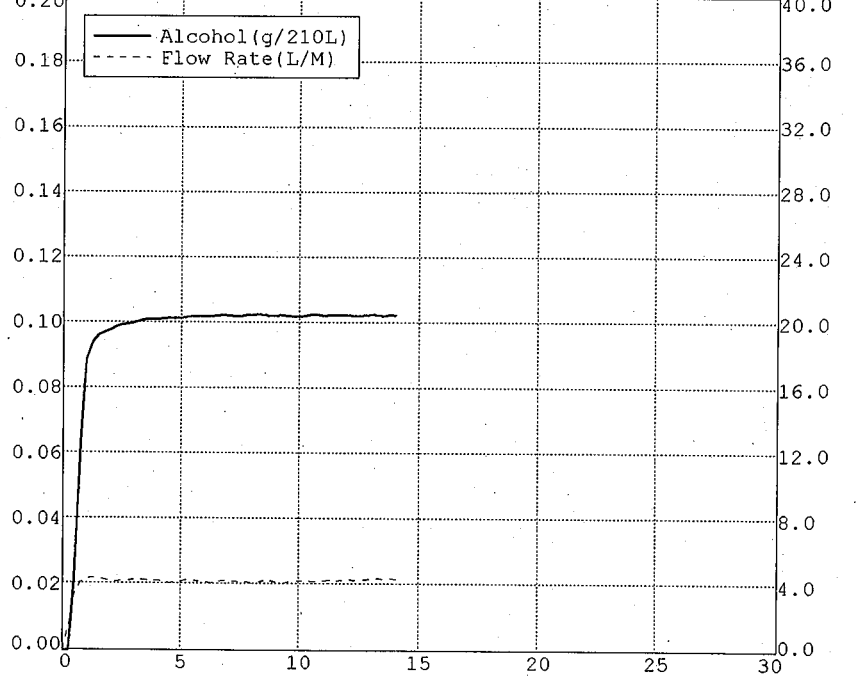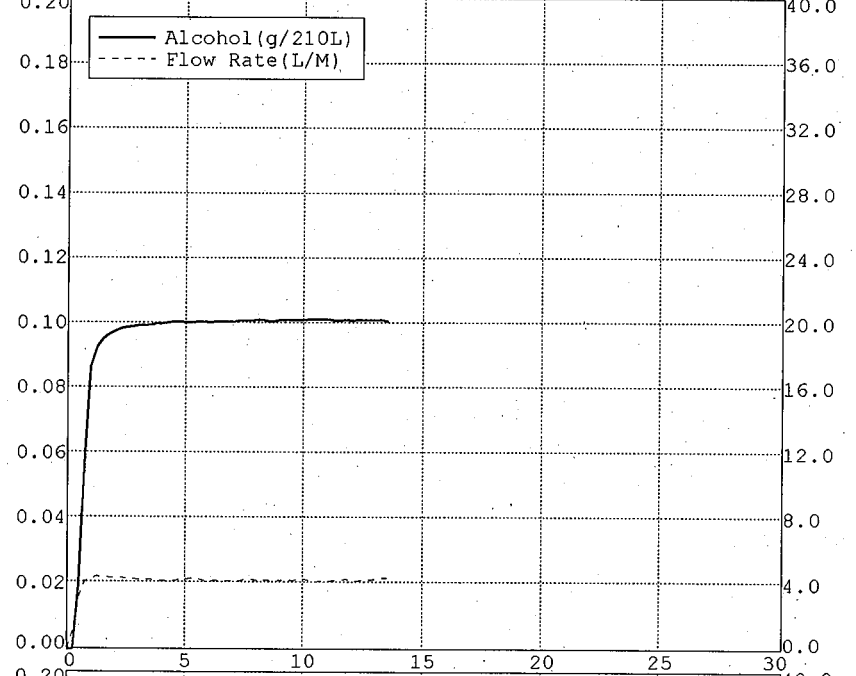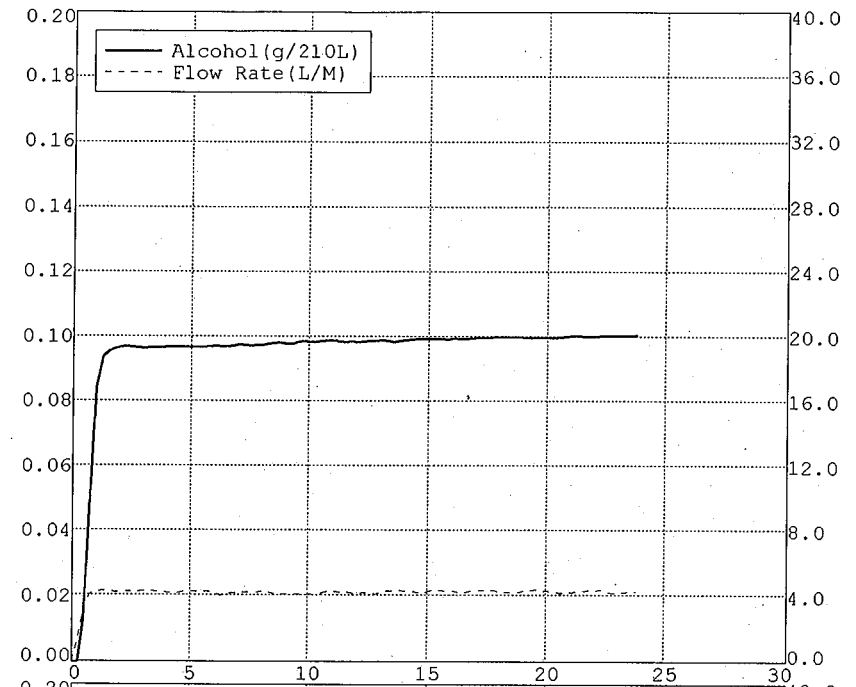

SOLUTION CHANGE

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282

Date: 02/03/2020

RMS
20-3734

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:21
INTERNAL STANDARD	VERIFIED	09:21
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:21
BLANK TEST	0.00	09:22
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:22
BLANK TEST	0.00	09:23
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:23
BLANK TEST	0.00	09:24

