

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 107308




Date: 12/26/2019

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19250

QM
19-1/84/89

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:04
INTERNAL STANDARD	VERIFIED	10:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:05
BLANK TEST	0.00	10:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:06
BLANK TEST	0.00	10:07
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:07
BLANK TEST	0.00	10:08

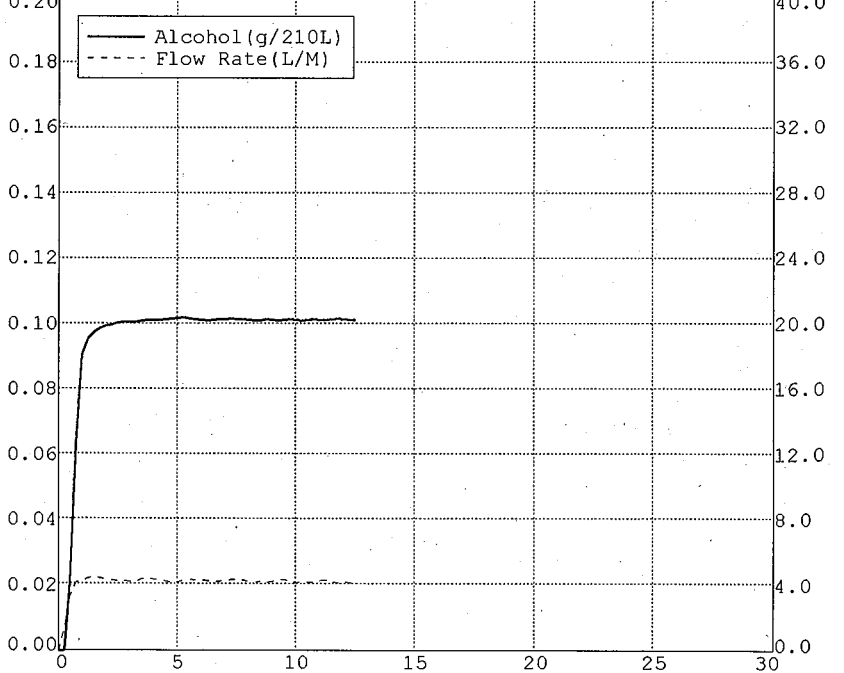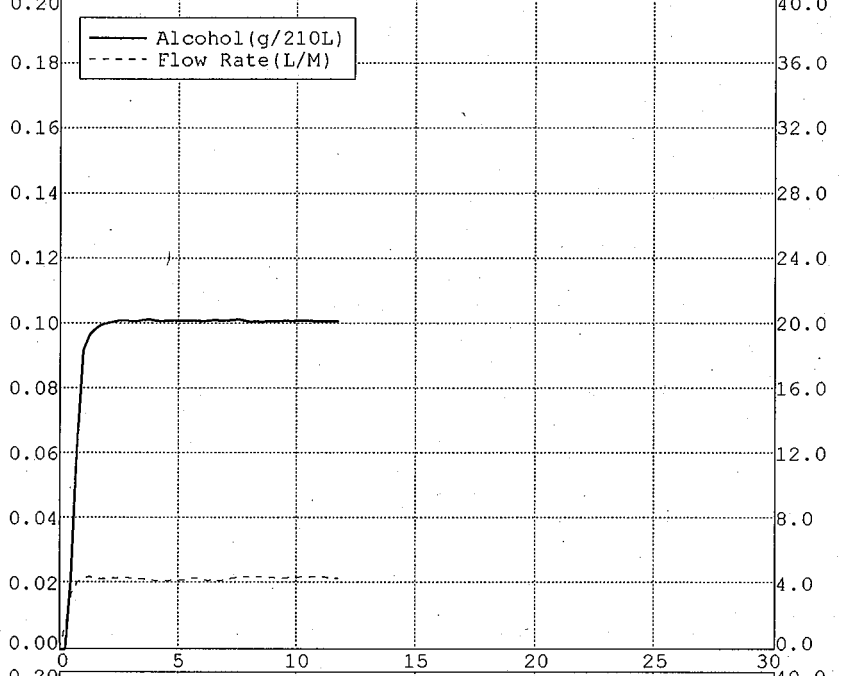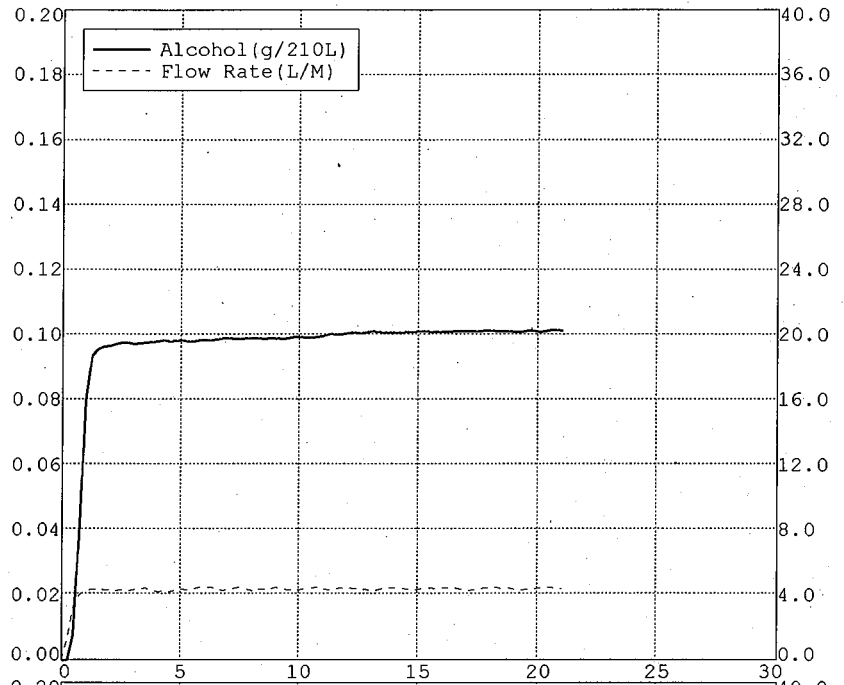

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282

Date: 12/26/2019

RM
1a-18189

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:33
INTERNAL STANDARD	VERIFIED	09:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:33
BLANK TEST	0.00	09:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:34
BLANK TEST	0.00	09:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:35
BLANK TEST	0.00	09:36

