

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 107308




CMJ
20-11/69

Date: 01/14/2020

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:32
INTERNAL STANDARD	VERIFIED	12:32
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:32
BLANK TEST	0.00	12:33
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:34
BLANK TEST	0.00	12:34
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:35
BLANK TEST	0.00	12:36

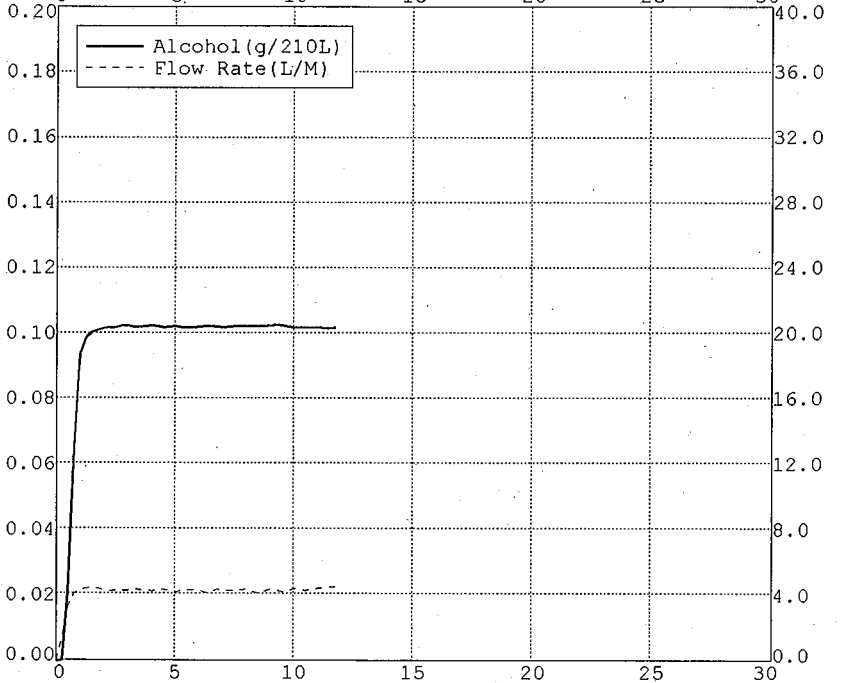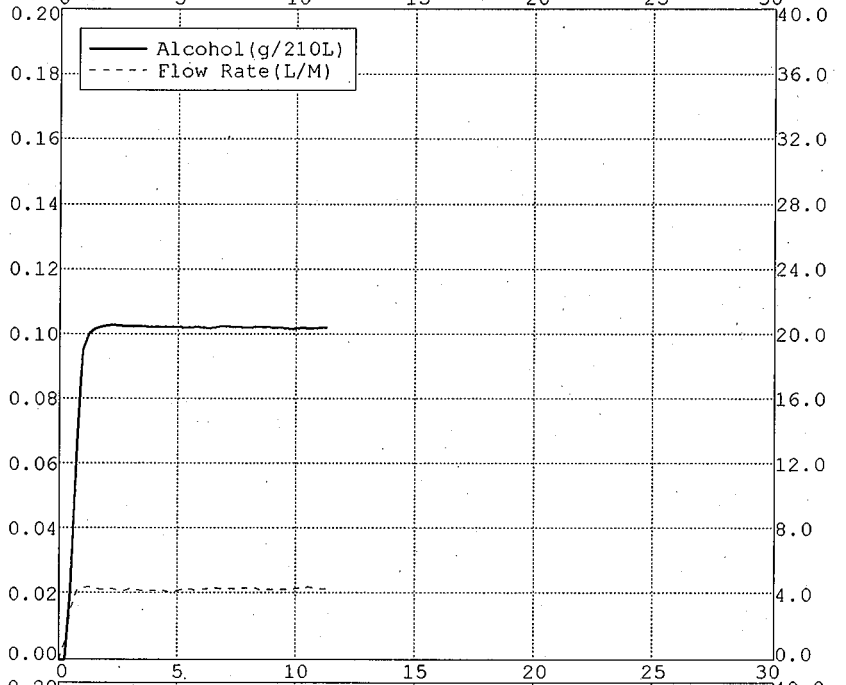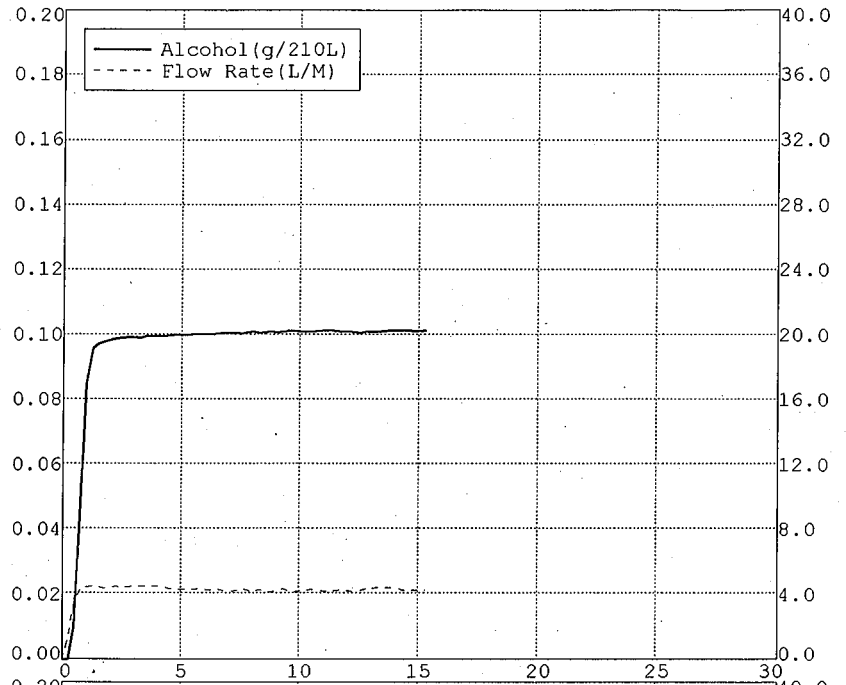

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282

Date: 01/14/2020

RMS
20-11/69

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:31
INTERNAL STANDARD	VERIFIED	12:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:31
BLANK TEST	0.00	12:32
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:33
BLANK TEST	0.00	12:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:34
BLANK TEST	0.00	12:34

