

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282




RMS
20-8181

Date: 03/10/2020

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 366682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:00
INTERNAL STANDARD	VERIFIED	09:00
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:00
BLANK TEST	0.00	09:01
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:01
BLANK TEST	0.00	09:02
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:02
BLANK TEST	0.00	09:03

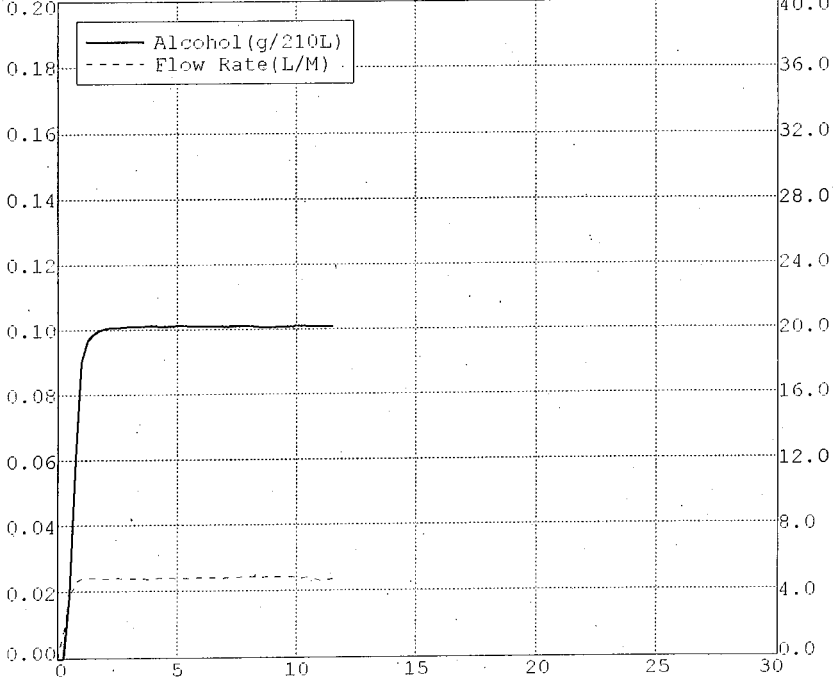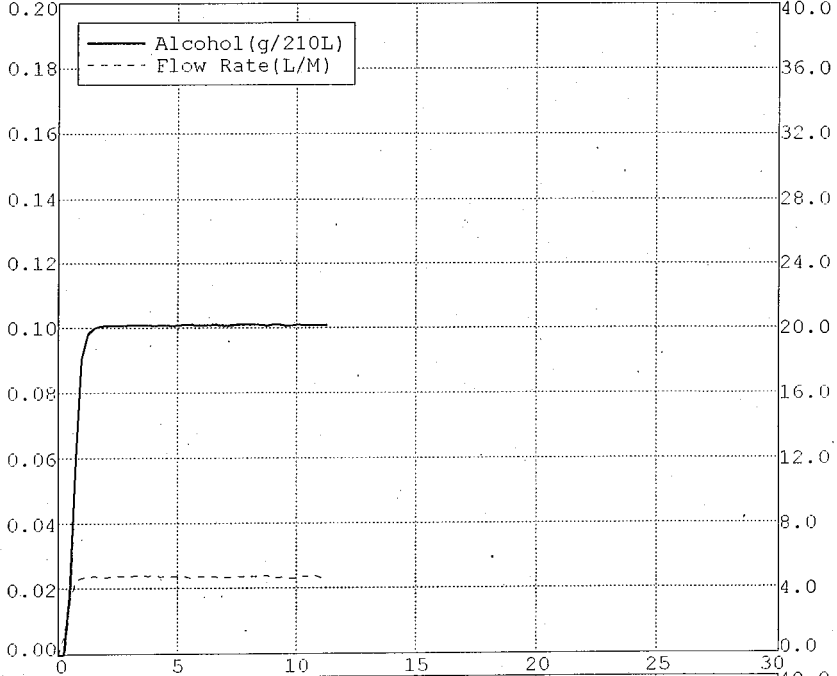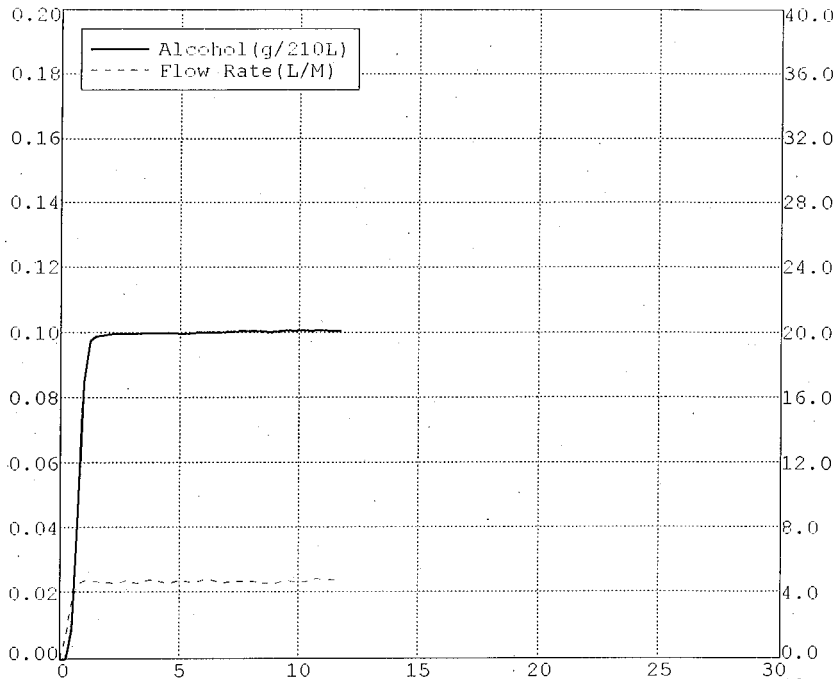

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 03/10/2020

*RMS
20-8181*

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:29
INTERNAL STANDARD	VERIFIED	09:29
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:30
BLANK TEST	0.00	09:31
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:31
BLANK TEST	0.00	09:32
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:32
BLANK TEST	0.00	09:33

