

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 03/24/2020

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19350

RMS
20-9769

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:55
INTERNAL STANDARD	VERIFIED	11:55
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:56
BLANK TEST	0.00	11:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:57
BLANK TEST	0.00	11:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:58
BLANK TEST	0.00	11:59

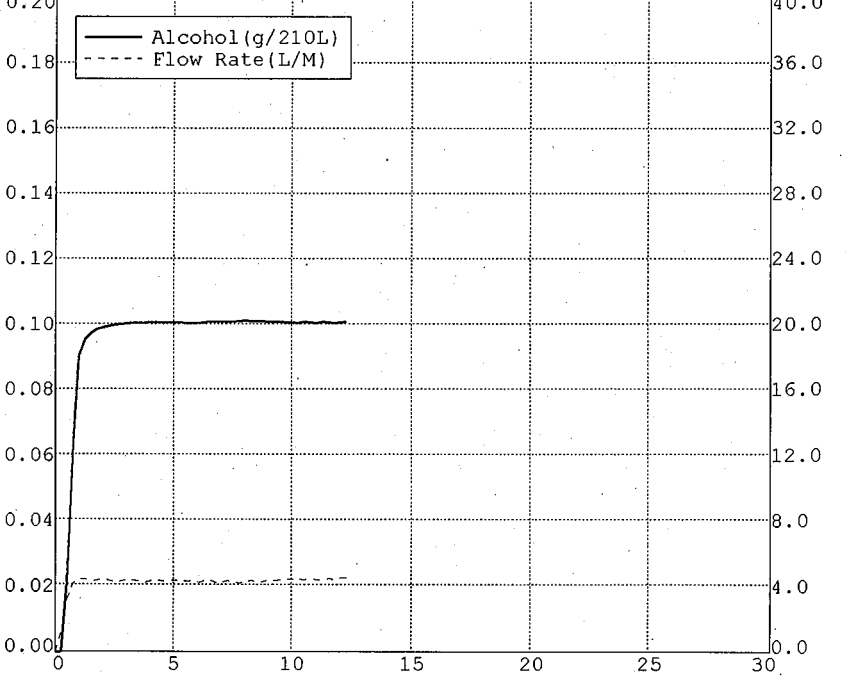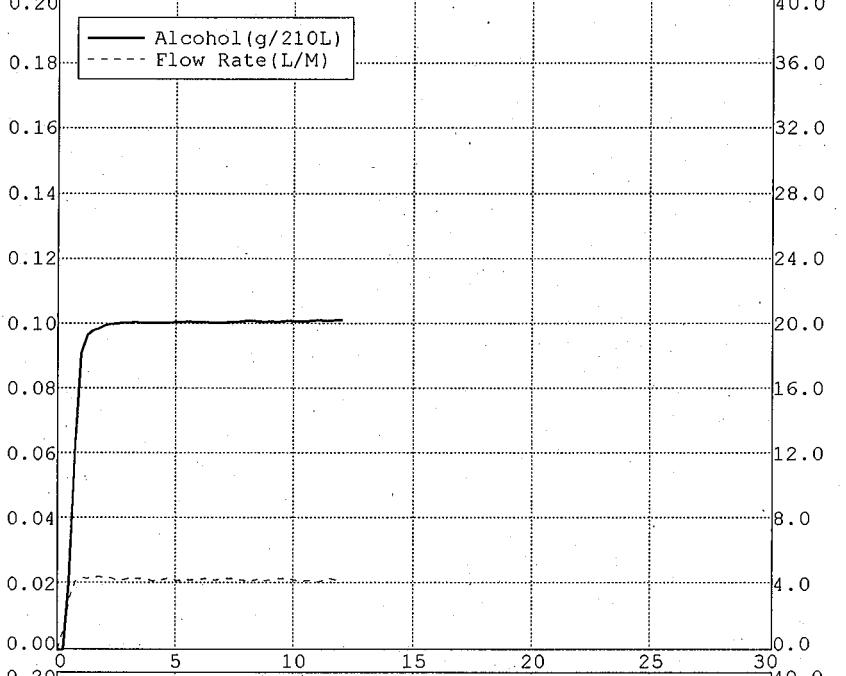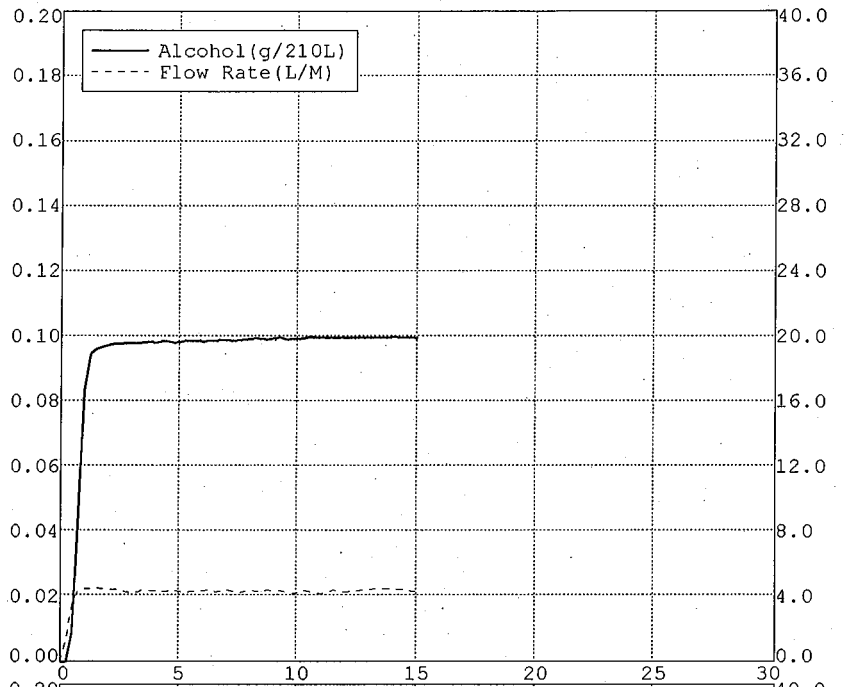

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282

Date: 03/24/2020

ZM >
20-9769

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:28
INTERNAL STANDARD	VERIFIED	11:28
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:28
BLANK TEST	0.00	11:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:30
BLANK TEST	0.00	11:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:31
BLANK TEST	0.00	11:31

