

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 03/31/2020

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19350

RMS
20-10594

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:22
INTERNAL STANDARD	VERIFIED	15:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	15:22
BLANK TEST	0.00	15:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	15:23
BLANK TEST	0.00	15:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	15:25
BLANK TEST	0.00	15:25

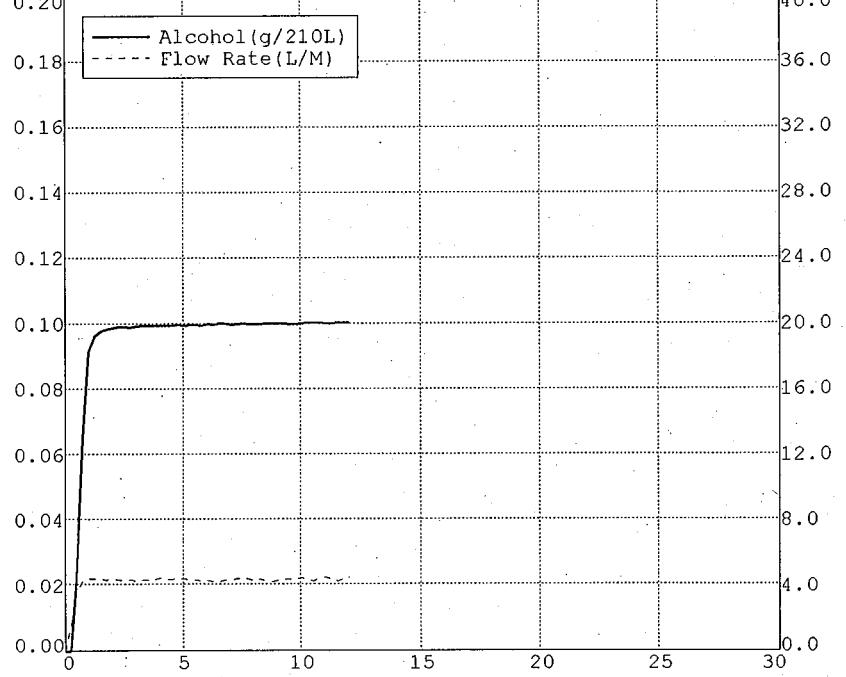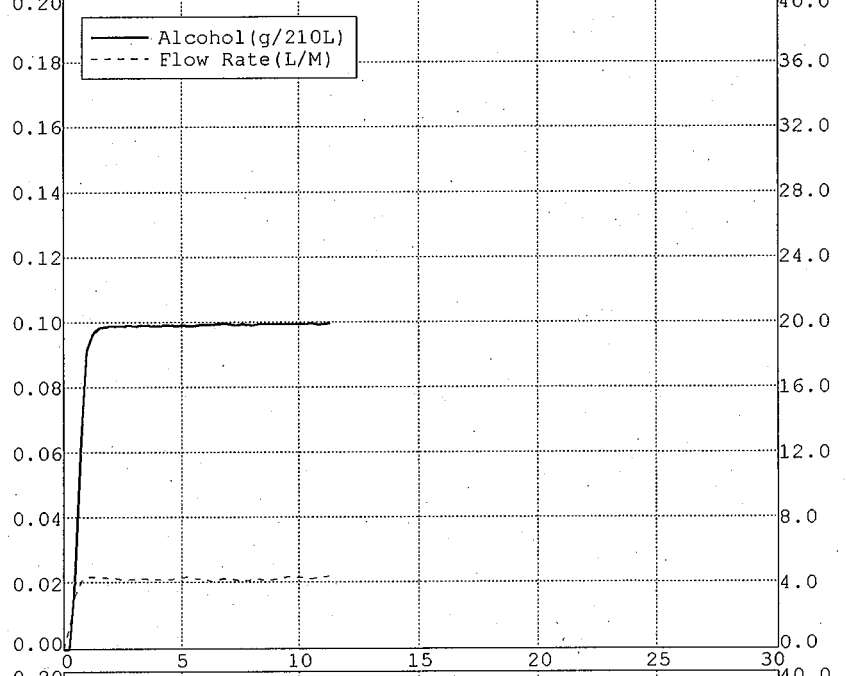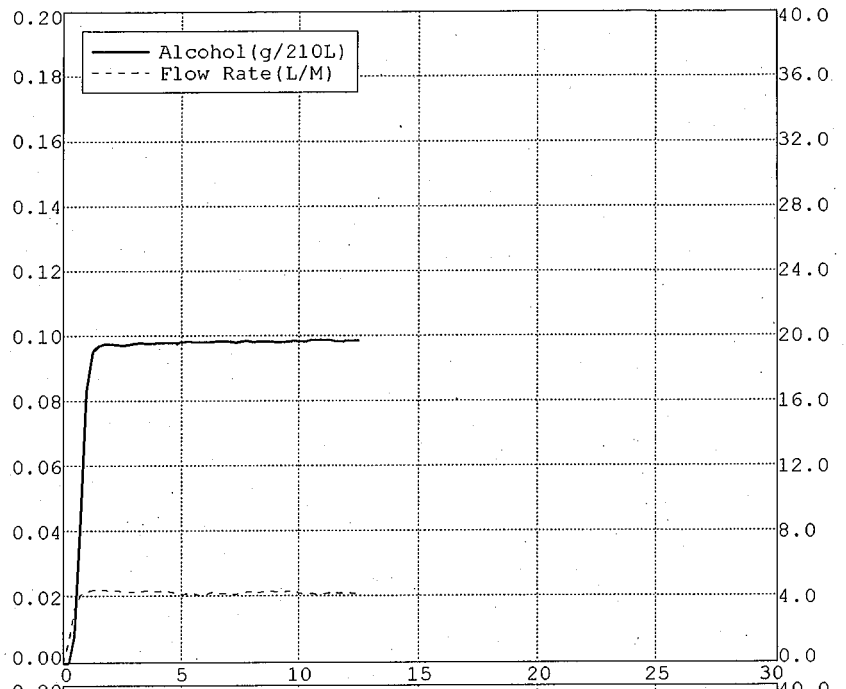

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282

Date: 03/31/2020

RMS
20-10594

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:51
INTERNAL STANDARD	VERIFIED	10:51
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:51
BLANK TEST	0.00	10:52
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:52
BLANK TEST	0.00	10:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:54
BLANK TEST	0.00	10:54

